

Takara Bio USA, Inc.

SmartChip® MultiSample NanoDispenser and SmartChip Dispenser Software User Manual

Cat. No. 640022, 640001
software v4.9
(101923)

Takara Bio USA, Inc.

2560 Orchard Parkway, San Jose, CA 95131, USA

U.S. Technical Support: technical_support@takarabio.com

United States/Canada
800.662.2566

Asia Pacific
+1.650.919.7300

Europe
+33.(0)1.3904.6880

Japan
+81.(0)77.565.6999

Page 1 of 78

Table of Contents

I.	Introduction	7
	A. Thank You for Your Order!	7
	B. About this Manual.....	7
	C. Technical Support	7
	D. SmartChip MultiSample NanoDispenser Safety Information.....	8
II.	System Description: Component Overview	9
	A. MultiSample NanoDispenser Specifications and Lab Requirements	13
	B. Setup and Installation.....	14
	C. Required Equipment and Supplies from Your Lab or Other Suppliers	14
	D. Required Materials from Takara Bio for All Applications	15
III.	System Description: SmartChip Technology.....	16
	A. Expression Analysis.....	16
	B. SNP Genotyping	17
	C. Software Files for Real-Time PCR Using the SmartChip System.....	17
	D. SmartChip Real-Time PCR Workflow Overview.....	19
IV.	Protocol: Quick Guide.....	20
V.	Protocol: Prepare the SmartChip MultiSample NanoDispenser (MSND)	21
	A. Power on the System.....	21
	B. Check System Containers	21
	C. Stream Check.....	23
	D. Refill the Pressure Reservoir.....	24
	E. Add Water to the Humidifier Reservoir.....	25
	F. Run the Daily Warmup	26
	G. Run the Tip Clean Procedure	28
VI.	Protocol: Prepare the Source Plates	29
	A. Prepare Source Plates for SmartChip MyDesign Chips.....	29
	B. Prepare Source Plates for Predispensed SmartChip Panels	31
	C. Prepare Source Plates Using Automation	32
VII.	Protocol: Configure the SmartChip MultiSample NanoDispenser (MSND)	32
	A. Chip Type Selector: Specify the SmartChip Type Being Used	32
	B. <i>Setup</i> Tab: Enter Information About Your Experiment	34
	C. <i>Sample Source Plate</i> Tab: Enter Your Sample Information	36

D. *Assay Source Plate* Tab: Enter PCR Assay Information (MyDesign Chips Only)..... 38

E. Generate and Save Your SmartChip Layout File..... 39

VIII. Protocol: Dispense Using the SmartChip MSND 40

 A. Place the Nanowell Chip in the SmartChip MSND 40

 B. Place the Source Plate in the SmartChip MSND 40

 C. Dispense into the Nanowell Chip..... 41

 D. Blot, Seal, and Spin the Chip 45

 E. Run PCRs on the SmartChip Cycler 47

 F. Clean the MSND 47

IX. Maintenance 47

 A. Daily Maintenance 47

 B. Shutdown Procedure 47

 C. Restart the SmartChip MSND from a Complete Shutdown 48

 D. Clean the Humidifier..... 48

 E. Verify the Dispensing Tip Alignment..... 48

 F. Remove Persistent Air Bubbles via Alcohol Wash Priming Procedure..... 51

 G. Common Replacement Parts 54

 H. Annual Preventative Maintenance 54

Appendix A. Troubleshooting..... 54

 A. On Startup of Software, Dewpoint Controller Error is Displayed 54

 B. Low Pressure Error Displayed 55

 C. Dispensing Head Does Not Home 55

 D. Low or Partial Dispenses 55

 E. Apparent Low Sample Concentration..... 56

 F. System Stalls Because the Syringe Does Not Move 56

 G. Persistent Soft Clicking..... 56

 H. Loud Digital Pressure Regulator Chattering..... 57

 I. Soft Clicking from the Digital Pressure Regulator, Fluid Leak Observed..... 57

Appendix B: Preparing Source Plates 57

 A. Preparing Source Plate Files in a Text Editor 57

 B. Workflow Guidelines for 768-Sample Dispense (MyDesign)..... 61

 C. Guidelines for Partially Filled 384-Well Source Plates or Plates Filled by Automation 61

 D. Printable 384-Well Source Plate Maps 64

Table of Figures

Figure 1. The SmartChip MSND.	9
Figure 2. Pressure reservoir seated on the electronic scale.	10
Figure 3. Harness connecting the fluidic and stage modules.	10
Figure 4. Stage module in the environmental chamber.	11
Figure 5. Peristaltic pump control box.	11
Figure 6. Connections on the rear of the peristaltic pump control box.	12
Figure 7. SmartChip real-time PCR workflow overview.	19
Figure 8. Pressure reservoir.	21
Figure 9. Wash bottle.	22
Figure 10. Humidifier Reservoir.	22
Figure 11. The [Stream Check] button under the <i>Advanced</i> tab.	23
Figure 12. Example of a stream check.	23
Figure 13. Venting the helium (or argon).	24
Figure 14. Opening the top of the protective cover.	24
Figure 15. Filling the reservoir with water.	25
Figure 16. Unplugging the hose adapter from the humidifier reservoir.	25
Figure 17. Filling the reservoir with deionized water.	26
Figure 18. Closing the Reservoir.	26
Figure 19. [Daily Warmup] button in the Instrument preparation section.	27
Figure 20. Monitoring the fluidic module for trapped bubbles.	27
Figure 21. <i>Daily Warmup</i> runtime dialog box.	28
Figure 22. The [Tip Clean] button in the Manual Control section.	28
Figure 23. The Utilities > Select chip type workflow and <i>Chip Type Selector</i> dialog.	33
Figure 24. Finding the selected chip well volume.	33
Figure 25. <i>Setup</i> tab in the SmartChip Dispenser Software.	34
Figure 26. Mode list.	34
Figure 27. SmartChip dispense options for a 150 nl chip.	35
Figure 28. SmartChip dispense options for a 250 nl MyDesign chip.	35
Figure 29. SmartChip assays X samples layout options.	35
Figure 30. <i>Sample source plate</i> tab.	36
Figure 31. Loading a sample source plate file.	36
Figure 32. Sample View list.	37
Figure 33. Well information.	37
Figure 34. Increasing the width of a source plate grid column in MS Excel.	37
Figure 35. Assay source plate tab.	38
Figure 36. Loading an assay source plate file.	38
Figure 37. Assay View list.	39
Figure 38. Generating a SmartChip Layout file.	39
Figure 39. Placing the chip on the dispensing platform inside the stage module.	40
Figure 40. Sample source plate on the plate nest.	41
Figure 41. <i>Run</i> tab.	42
Figure 42. <i>Check Water Level</i> pop-up error message.	42
Figure 43. Pop-up displayed when the system is adjusting the humidity of the environmental chamber prior to dispense.	43
Figure 44. Pop-up displayed when customer selects [Stop Waiting] in the pop-up shown in Figure 43.	43
Figure 45. Dispense button behavior in the <i>Run</i> tab for the default (ordered) dispense.	44

Figure 46. Where to find the "Allow Unordered Dispense" check box in the *Advanced* tab. 44

Figure 47. Dispense button behavior in the *Run* tab for an unordered dispense..... 44

Figure 48. Removing the backing from the SmartChip cycling film..... 45

Figure 49. Placing the cycling film on the chip. 46

Figure 50. Chip spinner and plate (left) and balance plate (right). 46

Figure 51. Sealing the alignment chip with alignment chip film..... 49

Figure 52. Positioning the sealed alignment chip on the SmartChip MSND..... 49

Figure 54. Alignment verification run results..... 51

Figure 55. Venting the noble gas from the pressure reservoir..... 52

Figure 56. Removing the reservoir cap and tubing..... 52

Figure 57. Fluidic harness..... 53

Figure 58. Elapsed time dialog box..... 53

Figure 59. "Unable to start dewpoint controller" *SmartChip Dispenser Error* pop-up message..... 54

Figure 60. The [Dispense Plate 1 Samples] button on the *Run* tab for the 6 assays X 768 sample layout..... 61

Figure 61. A 384-well plate containing 67 samples as will be dispensed using automation..... 62

Figure 62. A 384-well plate containing 67 samples with the MSND aspiration grid overlaid..... 63

Figure 63. The 384-well source plate fill map for 67 samples to accommodate the SmartChip MSND best practice..... 63

Figure 64. Printable 384-well plate map for dispense of 3 samples into a predisposed chip for gene expression panels. . 64

Figure 65. Printable 384-well plate map for dispense of 6 samples into a predisposed chip for gene expression panels. . 65

Figure 66. Printable 384-well plate map for dispense of 12 or 16 samples or 12 assays..... 65

Figure 67. Printable 384-well plate map for dispense of 20 samples..... 66

Figure 68. Printable 384-well plate map for dispense of 24 samples or assays..... 66

Figure 69. Printable, partial 384-well plate map for dispense of 36 samples or assays..... 67

Figure 70. Printable 384-well plate map for dispense of 42 samples into a predisposed SNP genotyping chip..... 67

Figure 71. Printable, partial 384-well plate map for dispense of 48 samples or assays..... 68

Figure 72. Printable, partial 384-well plate map for dispense of 54 samples or assays..... 68

Figure 73. Printable, partial 384-well plate map for dispense of 64 or 96 samples or assays..... 69

Figure 74. Printable, partial 384-well plate map for dispense of 72 samples or assays..... 70

Figure 75. Printable, partial 384-well plate map for dispense of 80 assays..... 70

Figure 76. Printable 384-well plate map for dispense of 108 samples..... 71

Figure 77. Printable 384-well plate map for dispense of 120 assays into a MyDesign chip..... 72

Figure 78. Printable 384-well plate map for dispense of 144 samples or assays into a MyDesign chip..... 73

Figure 79. Printable 384-well plate map for dispense of 216 samples or assays..... 74

Figure 80. Printable 384-well plate map for dispense of 248 assays into a MyDesign chip..... 75

Figure 81. Printable 384-well plate map for dispense of 296 assays into a MyDesign chip..... 76

Figure 82. Printable 384-well plate map (blank)..... 77

Table of Tables

Table 1. User manual symbols and conventions..... 7

Table 2. MSND specifications and lab requirements..... 13

Table 3. SmartChip MSND Starter Kit components..... 14

Table 4. Materials required for all applications..... 15

Table 5. Materials required for expression and genotyping analysis using SmartChip MyDesign Chips..... 15

Table 6. Materials required for expression and genotyping analysis using predisposed SmartChip Panels..... 16

Table 7. Master mixes to use with SmartChip applications..... 16

Table 8. Quick Start Guide.	20
Table 9. 384-well plate preparation for a 150 nl MyDesign chip	30
Table 10. 384-well plate preparation for a 250 nl MyDesign chip	30
Table 11. Sample source plates for gene expression analysis: predisensed SmartChip Panels.	31
Table 12. Sample source plates for SNP genotyping: predisensed SmartChip Panels.	32
Table 13. Selecting the correct sealing film to use on the nanowell chip for each SmartChip type.	45
Table 14. Determining the next step of the protocol after MSND dispense.	47
Table 15. Problem: On startup of software, dewpoint controller error is displayed (Figure 59).....	54
Table 16. Problem: Hanging drop, drop dispersion, or improper dispensing	55
Table 17. Problem: Low Pressure error displayed.	55
Table 18. Problem: Dispensing head does not home.	55
Table 19. Problem: Low or partial dispenses.....	55
Table 20. Problem: Apparent low sample concentration.	56
Table 21. Problem: System stalls because the syringe does not move.	56
Table 22. Problem: Persistent soft clicking.....	56
Table 23. Problem: Loud digital pressure regulator chattering.....	57
Table 24. Problem: Soft digital pressure regulator clicking and fluid leak observed.	57
Table 25. Attributes for sample source plate files for gene expression analysis.....	59
Table 26. Attributes for assay source plate files for gene expression analysis.	59
Table 27. Attributes for sample source plate files for SNP genotyping.....	60
Table 28. Attributes for assay source plate files for SNP genotyping.	60

I. Introduction

A. Thank You for Your Order!

Congratulations on the purchase of your SmartChip MultiSample NanoDispenser (MSND). The SmartChip MSND is designed to load samples into SmartChip Panels and to load both samples and real-time PCR assays or PCR primers into SmartChip MyDesign Chips.

B. About this Manual

This manual provides instructions for the safe operation and maintenance of the SmartChip MSND. This manual also includes instructions for using the SmartChip Dispenser Software.








NOTE: The SmartChip MSND has been qualified to work with either **helium** (preferred) or **argon** gas if helium is unavailable. References to 'noble gas' in this document should be interpreted to mean whichever of these two are being used in your system.

IMPORTANT: Other noble gases (neon, krypton, etc.) should NOT BE USED.

Symbols and conventions

The following symbols and conventions (Table 1) are used throughout this manual.

Table 1. User manual symbols and conventions.

Symbol	Description
	DANGER: Indicates a hazardous situation that could result in death or serious injury.
	WARNING: Indicates a potentially hazardous situation that could result in injury to the user or damage to or destruction of the system.
	CAUTION: Indicates a hazard that could result in loss of data or damage to the system.
	Indicates the presence of an electrical shock hazard. Proceed with caution. This symbol may appear next to either a WARNING or CAUTION symbol.
	Indicates the presence of a biological hazard. Proceed with caution. This symbol may appear next to either a WARNING or CAUTION symbol.
	Indicates the presence of a mechanical or pinch hazard. Proceed with caution. This symbol may appear next to either a WARNING or CAUTION symbol.
	IMPORTANT: Provides information on proper system operation.
NOTE:	NOTE: Provides helpful ancillary information to support the use of the system.

C. Technical Support

Review the information in this manual thoroughly before using the equipment. Also review documentation supplied with any accessory equipment you are using.

If you require additional assistance, contact Takara Bio [technical support](#).

D. SmartChip MultiSample NanoDispenser Safety Information



CAUTION: There are no user-serviceable parts inside the instrument. Service of any internal parts should be performed by a qualified Takara Bio service technician.

Operating conditions

The instrument is safe to operate with the covers in place. The covers protect the user from live parts and must not be removed during operation. If this equipment is not used as specified by the manufacturer, the protection provided by this equipment may be impaired.

Operate the SmartChip MSND only inside an appropriate building. Do not operate the SmartChip MSND outside or in wet environments.

Instrument use



WARNING: Use of the SmartChip MSND may cause exposure to toxic or biohazardous chemicals, thereby presenting a hazard. Wear appropriate personal protective equipment (PPE), which should, at minimum, include gloves, eye protection, and lab coat at all times in the laboratory.



WARNING: Class I Equipment: This equipment must be grounded. The power plug must be connected to a properly wired grounded outlet. An improperly wired outlet could place hazardous voltages on accessible metal parts.



CAUTION: Do not position the equipment so that it is difficult to operate the power switch or remove the power cord.



WARNING: Use only the power cord provided by the manufacturer. Do not replace the power cord with an inadequately rated cord.

Certification and standards information

The SmartChip MSND fulfills the following requirements: EN 61010-1:1993 + A2:1995/IEC 61010-1:1990 + A1:1992 + A2:1995.

Safety specifications are also met under the following environmental conditions, which are in addition to those stated in the operating conditions:

- **Installation Category (overvoltage category) II according to IEC 60664-1.** The Installation Category defines the level of transient overvoltage which the instrument is designed to withstand safely. It depends on the nature of the electricity supply and its means of overvoltage protection. For example, in CAT II, which is the category typically used for instruments in hospital, research, and industrial laboratories, the expected transient overvoltage is 2,500 V for a 230-V supply and 1,500 V for a 120-V supply.
- **Pollution Degree 2 according to IEC 60664-1.** Pollution Degree 2 assumes that normally only nonconductive pollution (e.g., dust) are present in the operating environment, with the exception of occasional conductivity caused by condensation.

Both the Installation Category (overvoltage category) and the Pollution Degree affect the dimensioning of electrical insulation within the instrument.

Moving and lifting the system



WARNING: If you need to move the system after it has been installed, use proper lifting techniques and appropriate moving equipment. More than one person may be required, particularly when moving the stage module.

Warning labels on the instrument

Please note the warning label on the instrument.



WARNING: This system contains moving parts. Keep hands away from the system while the instrument is in use.

II. System Description: Component Overview

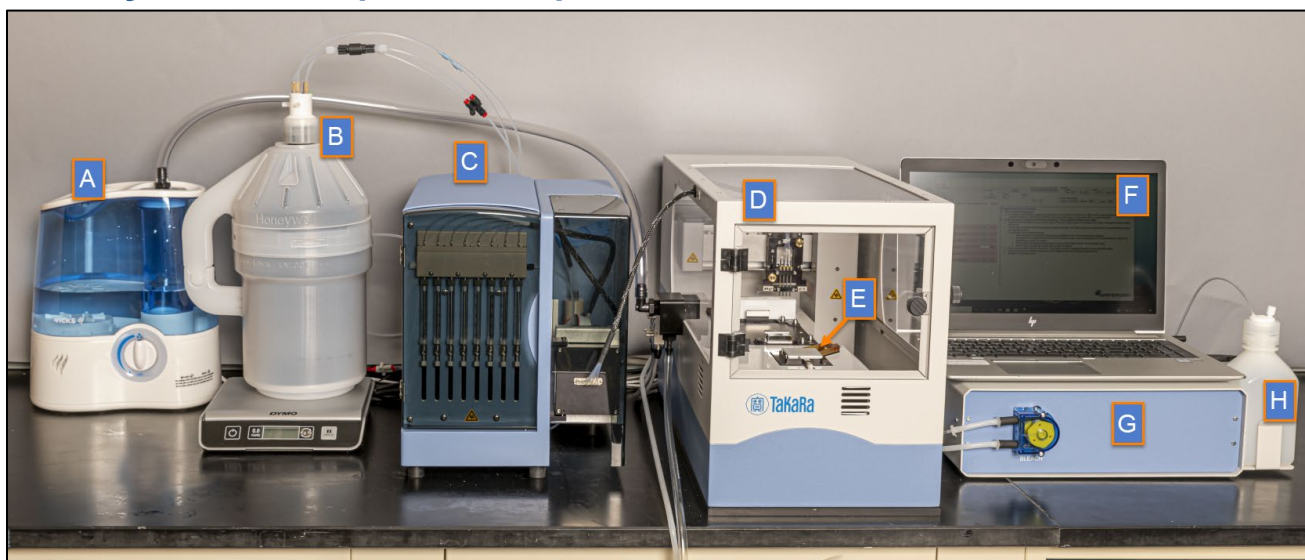


Figure 1. The SmartChip MSND.

The SmartChip MSND includes the following components:

- A. Humidifier
- B. Pressure reservoir and electronic scale
- C. Fluidic module
- D. Environmental chamber
- E. SmartChip stage module
- F. Laptop computer
- G. Peristaltic pump control box
- H. Wash bottle
- I. Waste container (not shown)

Other items not shown include the fluidic harness and power cord, waste container, SmartChip Dispenser Software, user manual (this document), digital pressure regulator (DPR), tool set, blotter, chip spinner and balance plate, and SmartChip Source Plate Layout Guides.

Pressure reservoir and electronic scale

The pressure reservoir contains pressurized (by helium or argon), deionized, degassed, filtered water that occupies all fluid paths in the fluidic module. The liquid is used to draw and push air gaps and reagents through the harness and tip. The pressure reservoir sits on an electronic scale (Figure 2) which monitors water level so that users can make sure there is enough water prior to starting a chip-dispense operation.

NOTE: On some instruments, the electronic scale will automatically shut off after a period of inactivity as a power-saving measure. Please check that the scale is on before each use. If it is not, remove the reservoir bottle from the scale and push the power button (located on the front-left of the instrument in Figure 2, below). Once the scale is tared, place the bottle back on the scale.



Figure 2. Pressure reservoir seated on the electronic scale.

Humidifier

The humidifier maintains the relative humidity in the stage module to minimize reagent evaporation during the dispensing process.

Fluidic module

The fluidic module is a hydro-pneumatic system that controls the aspiration and dispensing of samples and reagents in the stage module. A single interface cable, called a tubular harness, facilitates the mechanical control between the fluidic and stage modules (Figure 3). Noble gas pressure and solenoid valves are used to control liquid dispensing. The fluidic module also regulates the noble gas to the pressure reservoir through a digital pressure regulator.

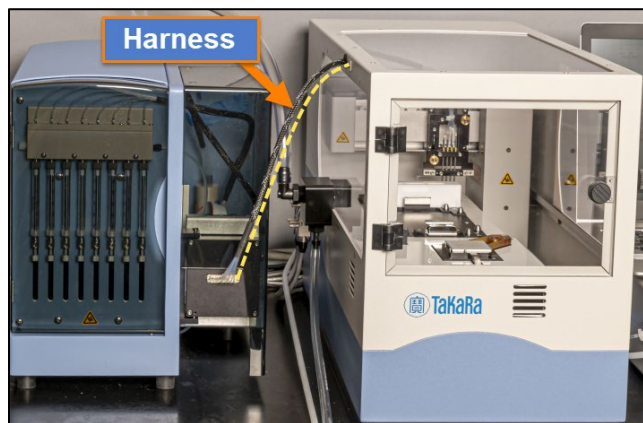


Figure 3. Harness connecting the fluidic and stage modules. The harness (black) is highlighted by the yellow-dashed line in the figure.

SmartChip stage module

The stage module houses the head, tips, SmartChip dispensing platform, plate nest, wash station, and tip mount used for aspirating reagents and dispensing them into a MyDesign chip (Figure 4). An environmental chamber surrounds the stage module to maintain optimal humidity levels during reagent dispensing.

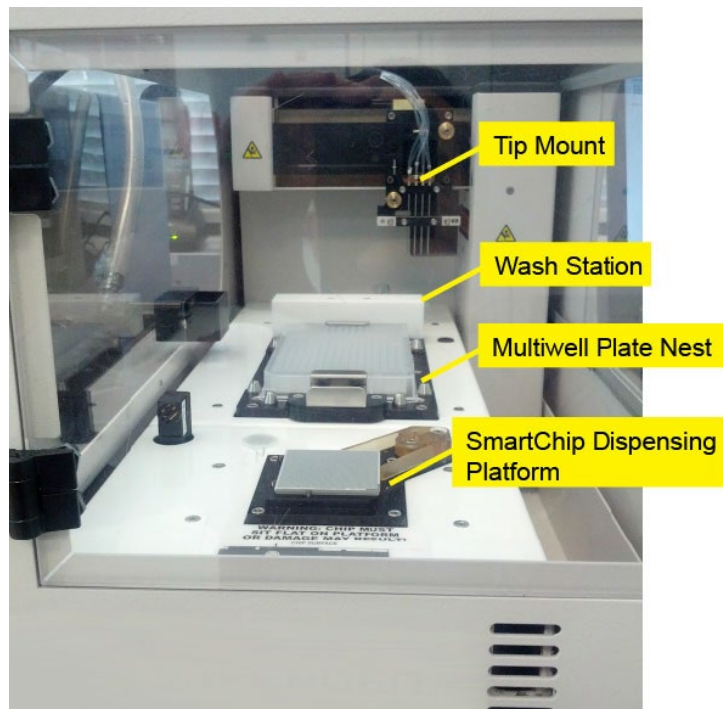


Figure 4. Stage module in the environmental chamber.

Peristaltic pump control box and environmental controller

The peristaltic pump control box includes one peristaltic pump, which pumps and drains wash solution into the SmartChip MSND and out to the waste container during the tip washing cycles. The peristaltic pump control box is connected to the fluidic module through two of the module's I/O channels.

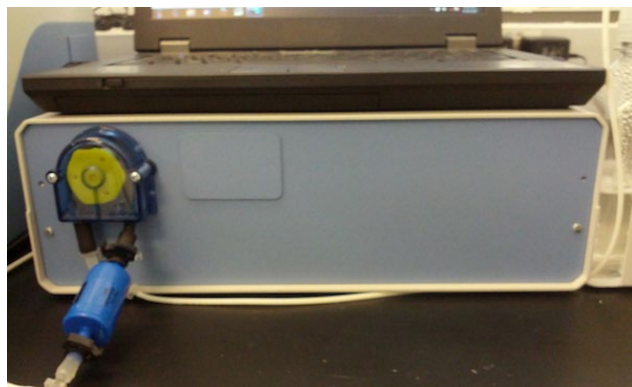


Figure 5. Peristaltic pump control box.

There are two PI controllers inside the pump control box that monitor the enclosure temperature, relative humidity (RH), and chip temperature. They adjust the RH and chip temperature to minimize evaporation during sample dispensing.

The rear of the pump control box has the connections to other components of the system, as shown below (Figure 6).



Figure 6. Connections on the rear of the peristaltic pump control box.

The connections, starting from the top left, are:

- **I/O:** connection to the peristaltic pump
- **TEC:** connection to the stage module
- **VACUUM:** connection to the helium (or argon) supply
- **SENSORS:** connection to the temperature and humidity sensors in the stage module
- **MSND 1:** connection to the fluidic module
- **MSND 2:** connection to the fluidic module
- **SCALE:** connection to the electronic scale
- **COMPUTER:** USB connection to computer
- **HUMIDIFIER:** power connection to the humidifier

Wash bottle

The wash bottle contains 0.2% hypochlorite solution, which is used during the tip cleaning steps of the dispensing protocol to prevent cross-contamination. The hypochlorite solution is pumped through tubing from the reservoir to the wash stage through a mini-peristaltic pump.

A. MultiSample NanoDispenser Specifications and Lab Requirements

Table 2. MSND specifications and lab requirements.

Category	Specification
Dispense volume	50 nl or 100 nl per nanowell
Software	SmartChip Dispenser Software
Laptop computer	Windows 10, 2 GB memory, 120 GB storage, 1 GB network adapter, USB ports for memory sticks
Power requirements (for different power supply types)	<p>120 VAC/60 Hz mains: one 120-V, 15- or 20-A circuit. Three NEMA 5–15 receptacles are required for the fluidic module, pump box, and laptop computer. (The humidifier plugs into the pump box, and thus a separate receptacle is not required.)</p> <p>220–240 VAC/50 Hz mains: one 10-A circuit to power a 230:115 step-down transformer and NEMA 5–15 power strip (transformer and power strip are supplied with the system). Transformer adapters will be supplied for Continental Europe (Schuko type), UK, and China installations.</p> <p>100 VAC/50–60 Hz mains: one 15-A circuit to power a 100:120 step-up transformer and NEMA 5–15 power strip (transformer and power strip are supplied with the system). Transformer suitable for Japanese power receptacles.</p>
Fuses	Dispenser; 5 x 20 mm, T5H 1.6 watts/6.3 A max 250 V
Environmental conditions	<p>Ambient temperature: 15–30°C, max variation <10°C per hour</p> <p>Relative humidity, non-condensing: 30–70%, max variation <10% RH per hour</p> <p>Altitude: <2,000 m from sea level</p> <p>Pollution degree: 2 or less</p>
Dimensions	<p>Laptop computer: 13" W x 2" H x 10" D (35 cm x 5 cm x 25 cm)</p> <p>Fluidic module: 11" W x 13" H x 18" D (28 cm x 33 cm x 45 cm)</p> <p>Stage module: 11" W x 16" H x 24" D (27 cm x 40 cm x 60 cm)</p> <p>Peristaltic pump control box: 10" W x 15" H x 21" D (26 cm x 38 cm x 51 cm)</p>
Bench space	<p>Bench space required for dispenser, pump box, CPU, pressure reservoir, transformer (if required): 70" W x 30" D x 24" H (180 cm x 75 cm x 60 cm)</p> <p><i>Note: Bench space must be capable of supporting 110 pounds (50kg)</i></p>
Floor space	<p>Humidifier: 16" W x 32" H x 26" D (41 cm x 81 cm x 66 cm)</p> <p>Noble gas source: 10" diameter cylinder (or equivalent) x ~60" H (25 cm x 125 cm)</p> <p>Waste container: 8 3/4" W x 14 1/8" H x 6" D (22 cm x 36 cm x 15 cm)</p>
Weight	143 pounds (65 kg)
Performance	Takara Bio Standard Positive Control DNA Test: C _t SD <0.25
Run time	~50 to 80 minutes

B. Setup and Installation

Your Takara Bio Service Engineer will unpack and install your SmartChip MSND and explain the basic operation of the system. They will use material from the SmartChip MSND Starter Kit to qualify the instrument after installation and will leave reusable and/or remaining materials at your site. Table 3 below lists the SmartChip MSND Starter Kit components and Cat. Nos.

Table 3. SmartChip MSND Starter Kit components.

Component	Takara Bio Cat. No.
SmartChip Intermediate Film (pack of 10)	640031
SmartChip Cycling Film (pack of 10)	640033
Nanodispenser Alignment Chip (1)	640041
Nanodispenser Alignment Chip Film (pack of 10)	640030
Blotting Paper (pack of 10)	640021
SmartChip MSND Tube Protection Bags (pack of 10)	640034
Imitation Master Mix with UV Dye & ROX (45 ml)	640026
MSND 384-Well Source Plate and Seals (20 Pack)	640018
MSND 384-Well Source Plate and Seals (120 Pack)	640037

The computer that runs the SmartChip MSND is equipped for Wi-Fi access, but it is disabled. If you choose to activate Wi-Fi, we recommend that you seek support from your institution's IT personnel to avoid interfering with instrument operation.

NOTE: To avoid contaminating your PCR, do not install the SmartChip MSND in an area that could contain high-copy DNA or amplicons from previous PCR experiments.

C. Required Equipment and Supplies from Your Lab or Other Suppliers

Helium (or Argon)

- **Purity:** 99.9% or greater.
- **Capacity:** approximately 223 standard cubic feet (reported at 15.6°C and 1 atmosphere [1.01325 Bar]). This capacity is sufficient for six months or more of typical usage.
- **Pressure:** 2,264 psi (150 Bar), with a regulator with an inlet pressure from 0 to 280 psig (0–15 Bar). The outlet pressure should be set between 30 and 50 psi (2 Bar) using a regulator.
- **Fittings:** must accommodate the 3.2 mm outer diameter of the flexible urethane tube fittings (push-to-connect fittings). Acceptable thread forms are 1/8" NPT (female) or M5 straight thread (female).

Wash bottle

- ~500-ml container for 0.2% hypochlorite solution

Reagents for SmartChip MSND reservoirs

- **Pressure reservoir:** deionized, filtered water (Milli-Q or Elga system or equivalent; 0.2-µm filtration)
- **Wash bottle:** 0.2% hypochlorite (made from sodium hypochlorite in deionized, filtered water)

Other reagents and materials

- Prepared sample/PCR reagent mixtures. For SmartChip MyDesign Chips, you will also need PCR assays. Instructions for preparing samples and reagents for dispensing with the SmartChip MSND are provided.
- MyDesign Kits (Takara Bio, Cat. No. 640032 or 640036) or preprinted SmartChip Panels*

NOTE: TE panels have been discontinued.

- MSND 384-Well Source Plate and Seals (Takara Bio, Cat. No. 640018 or 640037)
- (For RNA analysis) RNase-OFF™ solution (Takara Bio, Cat. No. 9037)
- DNA decontamination solution such as DNAzap (Thermo Fisher Scientific, Cat. No. AM9890)
- 70% isopropanol

*Please contact [customer service](#) or your Takara Bio sales representative if you are interested in ordering preprinted SmartChip Panels. Customers in North America can [find their sales representative](#) on our website.

Equipment

- Ice bucket and/or cold rack
- Calibrated pipettes and nuclease-free, aerosol-resistant tips (8-channel and repeating pipettes are very useful in this procedure)
- Vortex mixer
- Centrifuge with rotor capable of spinning microwell plates at 3,220g

D. Required Materials from Takara Bio for All Applications

To order, visit our website at takarabio.com or contact [customer service](#) or your local sales representative.

For all applications

Table 4. Materials required for all applications.

Cat. No.	Product name	Product size	Description
640018	MSND 384-Well Source Plate and Seals	Pack of 20	These specific 384-well plates are the required container for solutions that will be dispensed using the SmartChip MultiSample NanoDispenser
640037		Pack of 120	
640021	Blotting Paper	Pack of 10	Small round pieces of blotting paper ideally suited to blotting filled chips

For expression and genotyping analysis using SmartChip MyDesign Chips

Table 5. Materials required for expression and genotyping analysis using SmartChip MyDesign Chips.

Cat. No.	Product name	Product size	Description
640032	SmartChip MyDesign Kit	1 chip	All kits include empty SmartChip nanowell chips and enough blotting paper, intermediate film, and cyler sealing and pressure film for each chip in the kit. You add both nucleic acid samples and PCR assays using the SmartChip MSND.
640036		20 chips	
640253	SmartChip MyDesign Kit, 250nl	1 chip	
640031	SmartChip Intermediate Film	Pack of 10	(Optional) SmartChip sealing film used to temporarily seal chips between SmartChip MSND dispensing steps. Also included in the SmartChip MyDesign Kit.
640033	SmartChip Cycling Film	Pack of 10	Optical chip sealing film for real-time PCR cycling in the SmartChip cyler

For expression and genotyping analysis using predispensed SmartChip Panels

Table 6. Materials required for expression and genotyping analysis using predispensed SmartChip Panels.

Cat. No.	Product name	Product size	Description
Various	SmartChip Panel		Predispensed SmartChip Panels containing PCR assays. Custom and fixed-content SmartChip Panels are available. You add experimental samples and PCR reagents using the SmartChip MSND.
640033	SmartChip Cycling Film	Pack of 10	Optical chip sealing film for real-time PCR cycling in the SmartChip cycler

Takara Bio master mixes

Table 7. Master mixes to use with SmartChip applications.

Cat. No.	Product name	Product size	Description
640210	SmartChip TB Green® Gene	48 mL	Special intercalator dye-based formulation for gene expression studies
640211	Expression Master Mix	2.4 mL	
640208	SmartChip Probe qPCR	48 mL	Optimized for probe-based gene expression and SNP genotyping applications
640209	Master Mix	2.4 mL	

III. System Description: SmartChip Technology

SmartChip technology distinguishes Takara Bio's PCR platform from other systems. Each SmartChip has a 72 x 72 array of nanowells and can accommodate up to 5,184 150 or 250 nl real-time polymerase chain reactions (PCR) reactions in a single run. There are three types of chips:

- **SmartChip Panels 150 nl:** contain PCR assays dispensed into the chips at Takara Bio. You add your experimental samples and PCR reagents to these chips using the SmartChip MSND.
- **SmartChip MyDesign Chips 150 nl (blank):** You add experimental samples, PCR reagents, and PCR assays to these chips using the SmartChip MSND.
- **SmartChip MyDesign Chips 250 nl (blank):** You add experimental samples, PCR reagents, and PCR assays to these chips using the SmartChip MSND.

A. Expression Analysis

For mRNA expression analysis, the SmartChip Real-Time PCR System has been tested with cDNA from human brain (Cat No. 637242), human lung (Cat No. 637206), human placenta (Cat No. 637208), and a pooled reference sample (Cat No. 637260) with SmartChip TB Green® Gene Expression Master Mix (Takara Bio, Cat. No. 640210).

NOTE: Other master mixes have not been validated for performance and are not supported. Precipitate may be observed in the SmartChip TB Green Gene Expression Master Mix. This precipitate does not affect the performance of the kit. The precipitate can be dissolved easily by warming to room temperature and mixing for a few minutes. Ensure that the precipitate is fully dissolved before use.

- **SmartChip MyDesign Chips** are provided empty. Use the SmartChip MSND to add both PCR assay(s) and experimental cDNA or DNA sample(s) in any of the 14 configurations supported for expression analysis.

- **SmartChip Custom Panels** are designed for targeted expression analysis; they are custom manufactured to your specifications. Choose from commercially available assays or have your assay design of choice predispensed into a chip. We offer SmartChip Custom Panels for expression analysis in six different configurations, designed for analysis of 3–96 samples using 384–12 assays in quadruplicate.

B. SNP Genotyping

The SmartChip system can be used for SNP genotyping using TaqMan SNP Genotyping Assays (Thermo Fisher Scientific) with Minor Groove Binder (MGB), *BHQplus* assays (LGC Biosearch), rhAmp assays (IDT), and, with minor modifications, KASP assays (LCG Genomics). Please contact [technical support](#) if you have questions about implementing any of these assays.

- **SmartChip MyDesign Chips** are provided empty. Use the SmartChip MSND to add SNP genotyping assays, reagent master mix, and experimental DNA samples in any of the 14 configurations supported for SNP genotyping analysis.
- **SmartChip SNP Genotyping Panels** contain TaqMan SNP Genotyping Assays that you have shipped to Takara Bio. They are available in eight configurations to analyze 12–384 samples using a single replicate with 384–12 TaqMan SNP Genotyping Assays. We dispense the assays and send the resulting SmartChip SNP Genotyping Panels with a CD containing files with assay locations, thermal profile, and data analysis parameters. Use the SmartChip MSND to add your experimental DNA samples to the SmartChip Panel.

C. Software Files for Real-Time PCR Using the SmartChip System

The SmartChip Real-Time PCR System needs information about your experimental samples, your PCR assays, and how to run the PCRs. This section describes the information and files needed by the SmartChip MSND and the files created by the SmartChip Dispenser Software for use by the SmartChip cyclers.

1. Sample Information

The SmartChip MSND aspirates samples from a 384-well plate and dispenses them into the nanowells of the SmartChip Panel or MyDesign Chip. The SmartChip MSND requires that samples be located in specific wells, depending on the quantity of samples and the number of PCR assays. We refer to this plate as a "Source Plate".

You will need to enter sample information and locations into the SmartChip Dispenser Software; this information is stored in sample source plate files.

2. PCR Assay Information

The required PCR assay information varies depending on the type of chip you are using.

SmartChip MyDesign Chips

SmartChip MyDesign Chips are supplied empty. You add PCR assays and Sample/PCR reagent mixtures to the chips.

You will need to enter your PCR assay information and locations in the 384-well assay source plate into the SmartChip Dispenser Software; this information is stored in an assay source plate file.

- You can create assay source plate files by entering your PCR assay information and locations into the *Assay Source Plate* tab of the SmartChip Dispenser Software. If you are filling many SmartChip MyDesign Chips with the same set of PCR assays, you can open a saved assay source plate file that contains your assay set.
- If you are using an automated system to fill your assay source plates, you can prepare assay source plate files in a text editor. To simplify the process of entering the data, use the assay source plate template file corresponding to the SmartChip configuration you are using. (See Appendix A for instructions.)

Assay source plate files can include the following information:

- For gene or microRNA expression: assay names and IDs, amplicon melting temperature (T_m), and designation as a housekeeping assay
- For genotyping: assay names and IDs, gene, gene symbol, category ID, or species

Predisposed SmartChip Custom Panels (for genotyping or gene expression-based mRNA/microRNA expression)

Predisposed SmartChip Custom Panels contain the PCR assays that you've selected; the assay information is in protocol files on the CD that shipped with your SmartChip Panels. The protocol files contain the following PCR assay information for use by the qPCR software:

- **Assay Map file (.ga1 file):** PCR assay locations on the SmartChip Custom Panel
- **Assay Attributes file:**
 - For SmartChip Panels for mRNA or microRNA expression: assay names and IDs, amplicon melting temperature (T_m), and designation of reference assays
 - For SmartChip Genotyping Panels: information from the Assay Information File(s) (AIF) provided with the TaqMan SNP genotyping assay(s), such as each SNP assay allele information and specific cycle number relevant for the end-point cluster analysis for each run.

You do not need the protocol files to dispense samples into your chip, but you will need it to run your reactions on the SmartChip cyclers.

Predisposed SmartChip Panels (for mRNA, microRNA, or long noncoding RNA expression)

Predisposed SmartChip Panels contain a fixed set of PCR assays for gene expression or microRNA or long noncoding RNA analysis. The PCR assay information is in protocol files that are installed with the software. The protocol files contain the following PCR assay information for use by the qPCR software:

- **Assay Map file (.ga1 file):** PCR assay locations on the SmartChip Panel
- **Assay Attributes file:** assay names and IDs, amplicon melting temperature (T_m), and designation of reference assays

You do not need PCR assay information to dispense your sample into the chip, but you will need it to run your reactions on the SmartChip cyclers.

3. Files Generated by the SmartChip Dispenser Software

The SmartChip Dispenser Software creates an XML SmartChip Layout file (*.xml) from sample and PCR assay information you have entered. The file contains information about your samples and, if you are using a SmartChip MyDesign Chip, about the PCR assays in your chip. The SmartChip Layout file is required by the SmartChip cycler to run and analyze your experiment. (See "Generating and Saving Your SmartChip Layout File" in Section VII.D for more information.)

D. SmartChip Real-Time PCR Workflow Overview

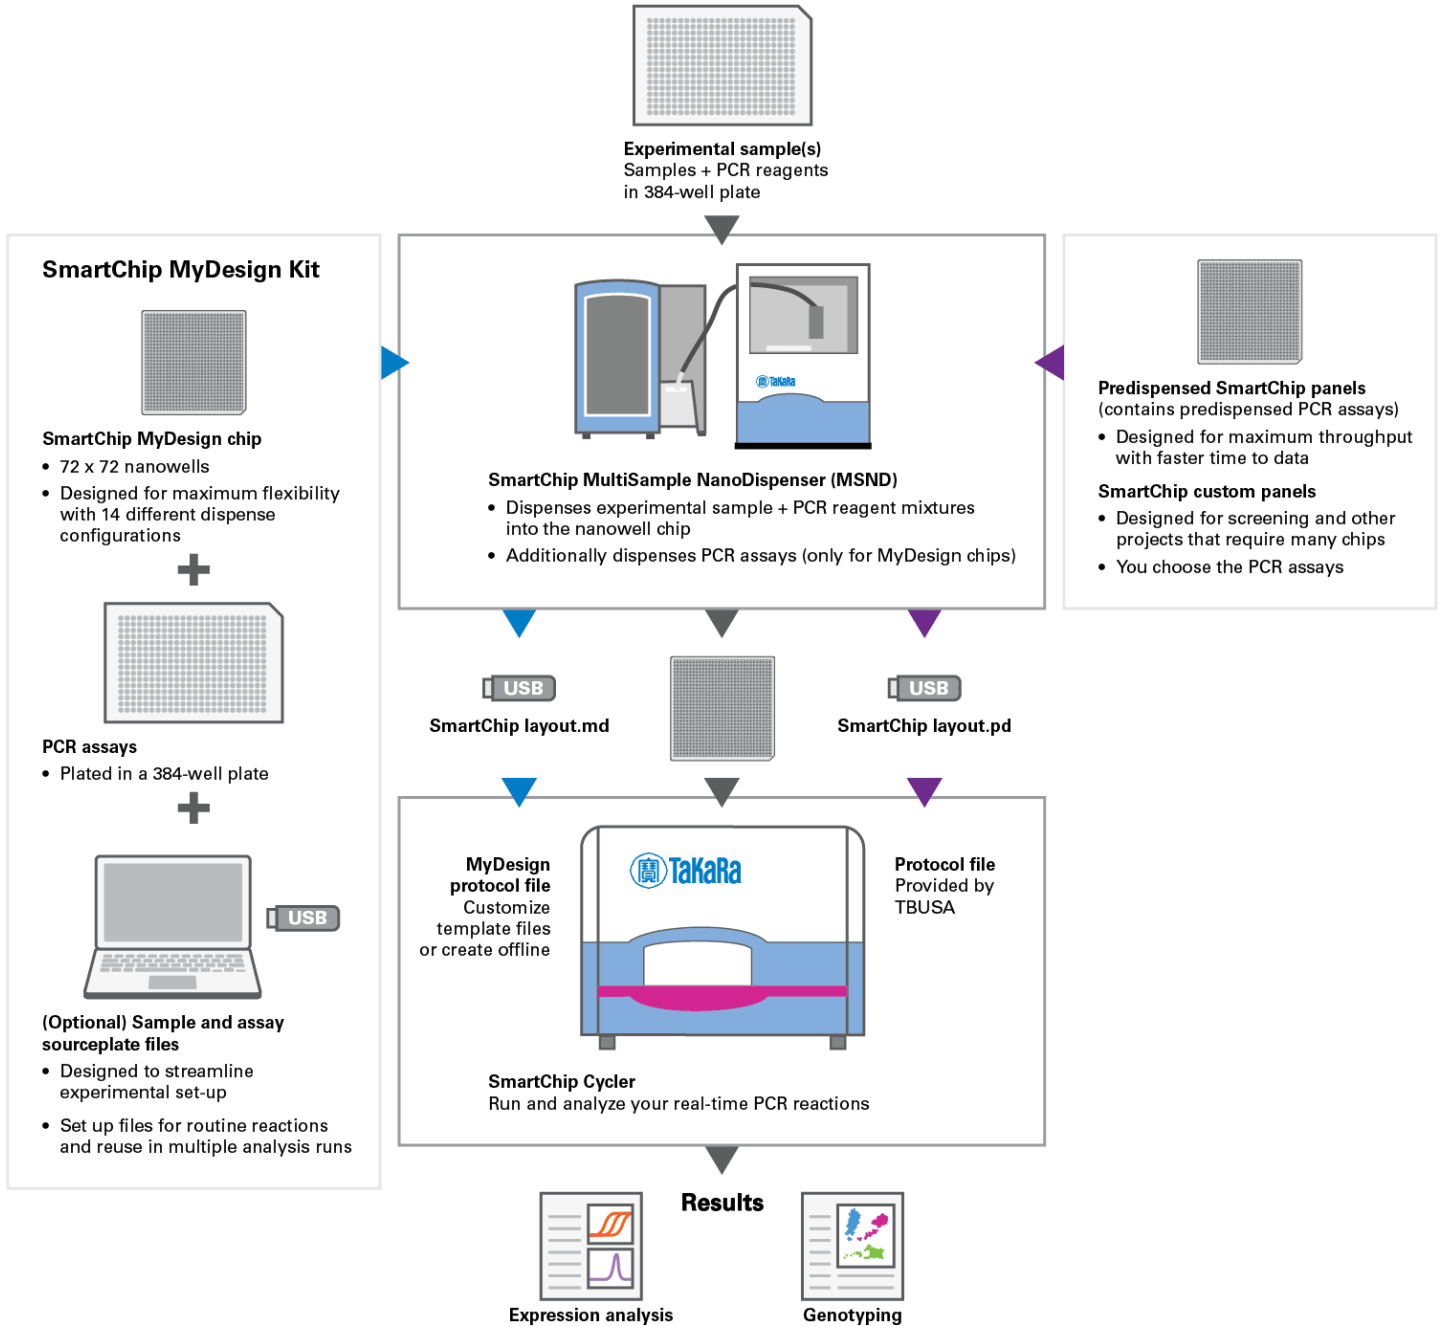


Figure 7. SmartChip real-time PCR workflow overview.

IV. Protocol: Quick Guide

Print the Quick Start Guide below (Table 8) for easy reference in the laboratory.

Table 8. Quick Start Guide.

For empty SmartChip MyDesign Chips

For predisposed SmartChip Panels

Prepare the SmartChip MultiSample NanoDispenser (MSND).

Prepare the Sample (and Assay) Source Plate(s).

For **SmartChip MyDesign Chips**:

1. Prep sample mixtures and plate in a 384-well plate
2. Dilute the PCR assays and plate in a 384-well plate

For predisposed **SmartChip Panels**:

1. Prep sample mixtures and plate in a 384-well plate

Enter information about your experiment in the SmartChip Dispenser Software.

1. Specify the well volume of your chip (150 nl or 250 nl) in the *Chip Type Selector* window (**Utilities > Select chip type**)
2. On the *Setup* tab, enter information about your experiment.
3. On the *Sample Source Plate* tab, enter your sample information. Open a sample source plate file from an earlier experiment, enter sample information by typing or copying from Excel, or import a file you created from a sample layout template.
4. On the *Assay Source Plate* tab, enter sample information as necessary

For **SmartChip MyDesign Chips**:

- Reuse an assay source plate file, enter assay information by typing or copying from Excel, or import an assay layout file

For predisposed **SmartChip Panels**:

- No action is required (**SmartChip Panels** contain predisposed PCR assays)

5. Click the [Generate SmartChip Layout File] button to create the layout file for the SmartChip cycler. Save it to a USB memory stick or network drive so that you can access it from the thermal cycler.

For **SmartChip MyDesign Chips**:

- A `SmartChip Layout.md` file is created

For predisposed **SmartChip Panels**:

- A `SmartChip Layout.pd` file is created

Dispense into your SmartChip Panel or MyDesign Chip.

6. Place the chip and sample source plate into the instrument and dispense samples and PCR reagents by going to the *Run* tab and clicking on the [Dispense Samples] button.

For **SmartChip MyDesign Chips**:

- a. Seal the chip with SmartChip Intermediate Film and centrifuge briefly
- b. Place your assay source plate into the instrument and dispense PCR assays into the chip by going to the *Run* tab and clicking on the [Dispense Assays] button
- c. Seal with SmartChip Cycling Film and centrifuge

For predisposed **SmartChip Panels**:

- Seal the chip with SmartChip Cycling Film and centrifuge

Run your PCRs on the SmartChip cycler. (See the [SmartChip Real-Time PCR System / SmartChip qPCR Software User Manual](#) for instructions.)

V. Protocol: Prepare the SmartChip MultiSample NanoDispenser (MSND)

A. Power on the System



IMPORTANT: Make sure that the Pump Box is connected to the proper USB port on the computer with a USB cable.

1. Power on the fluidic module and the pump box using the switches on the back of the components.
2. Power on the computer and start the SmartChip Dispenser Software. It may take ~5 min for the SmartChip MSND dew point sensors to stabilize and the system to become available.

B. Check System Containers

1. Check the noble gas tank pressure. The regulator should have a supply input (on the side closer to the noble gas tank) of >500 psi (3.5 MPa) and an output (on the side closer to the SmartChip MSND) of ~30–40 psi (0.24 MPa). If the noble gas tank pressure drops below 500 psi, replace the tank.
2. Check the amount of water in the pressure reservoir as described below.
 - a. Open the top of the protective cover on the pressure reservoir (Figure 8). Be careful not to misplace the O-ring or damage the tubes coming from the lid.

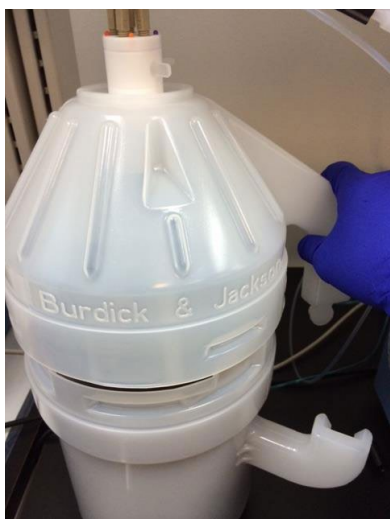


Figure 8. Pressure reservoir.

- b. Tilt the bottle sideways to check the amount of water in the reservoir. It should be at least half full of deionized filtered water at the beginning of a run.
 - c. If needed, add water to the reservoir (see "Refilling the Pressure Reservoir" in Section C below).
3. Check the waste container. If full, dispose of waste appropriately and replace the waste container with an empty one.
 4. Check the wash bottle. If there is less than ~1 inch (2.5 cm) of liquid in the wash bottle, add 0.2% reagent-grade sodium hypochlorite solution to the 500-ml mark (Figure 9). Replace the 0.2% sodium hypochlorite solution after three to five days. (If the bottle is exposed to direct sun light, change every three days.)

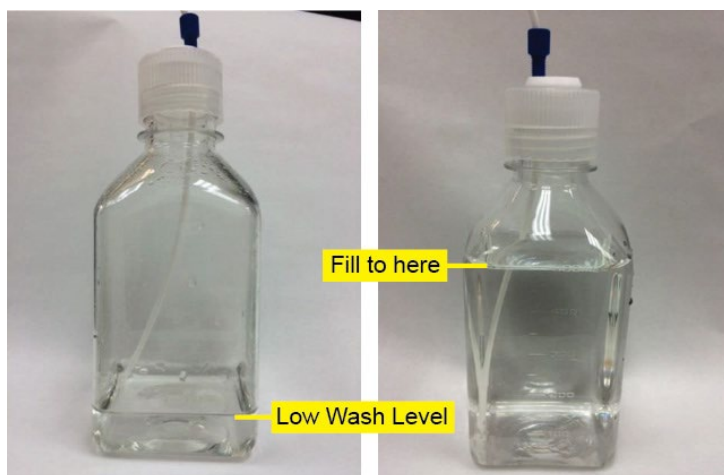


Figure 9. Wash bottle.

5. Check the humidifier reservoir. If the level of water in the humidifier reservoir is less than 2 inches (5 cm) from the bottom of the reservoir (Figure 10), add water (See "Adding Water to the Humidifier Reservoir" in Section V.D below).



Figure 10. Humidifier Reservoir.

6. Check the system humidity. Close all of the doors to the environmental chamber. Rotate the humidifier control switch all the way to the right (clockwise), to the maximum setting. For optimal performance, the humidity needs to be between 30–70%.
7. Perform the daily warmup. (See "Run the Daily Warmup" in Section V.E below.)
8. Perform the Tip Clean procedure. (See "Run the Tip Clean Procedure" in Section V.F below.)

C. Stream Check

1. Under the *Advanced* tab, click the [Stream Check] button.

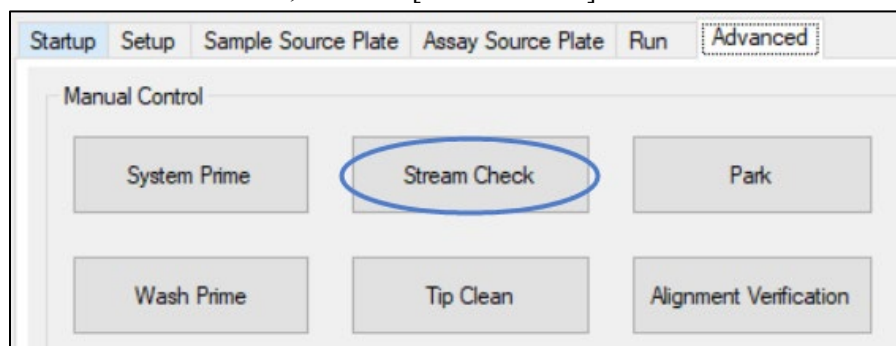


Figure 11. The [Stream Check] button under the *Advanced* tab.

NOTE: The other buttons on the *Advanced* tab located under the buttons shown in Figure 11 are reserved for use by a certified Field Service Engineer. Customers are discouraged from using these.

2. Observe the streams of fluid coming out of the tips to ensure they are relatively straight.

Figure 12 (below) illustrates an example of a stream check where one of the streams (tip C, third from the right) is not coming out straight, but at a sharp angle.

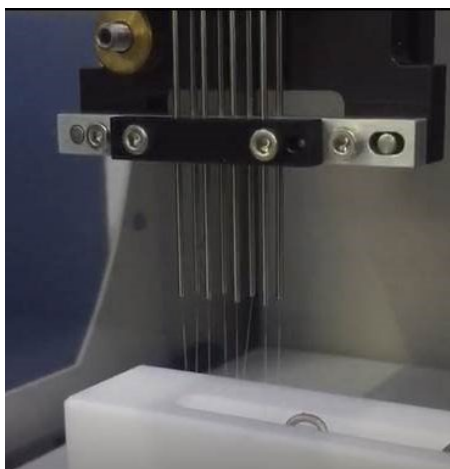


Figure 12. Example of a stream check. Tip C is streaming at an angle, indicating an issue that should be corrected to proceed.

If one or more streams is not straight, the following steps can be performed to try and correct it:

- a. Repeat the tip clean procedure (Section V.G) then the stream check procedure above, up to two times
- b. Perform an alcohol wash (Section IX.E)

If the steps above do not correct the problem, please contact [technical support](#) for further assistance.

D. Refill the Pressure Reservoir

1. Put on clean gloves.
2. Vent the noble gas by closing the stopcock on the noble gas input line and opening the vent stopcock (Figure 13).

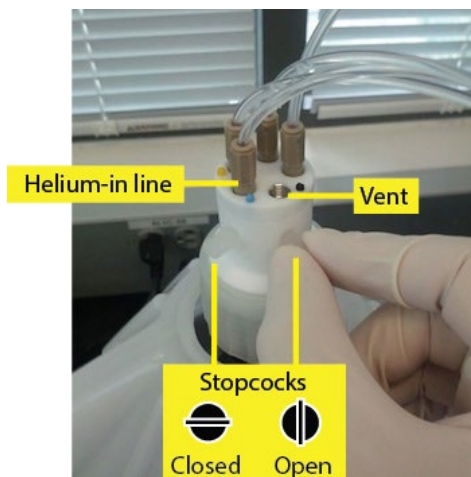


Figure 13. Venting the helium (or argon).

3. Open the top of the protective cover (Figure 14). There is no need to remove the entire tubing harness from the reservoir.

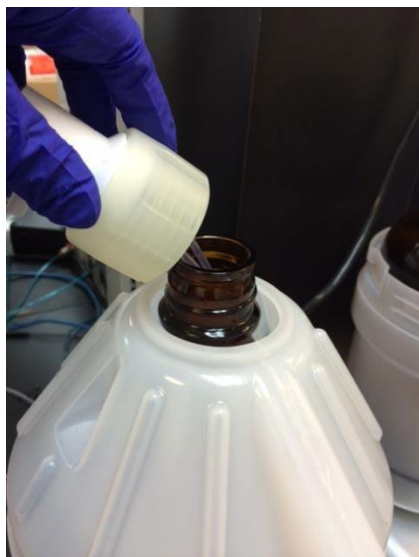


Figure 14. Opening the top of the protective cover.

- Using a graduated cylinder, fill the bottle with deionized, filtered water to the top of the lower part of the protective cover (Figure 15).



Figure 15. Filling the reservoir with water.

- Reattach the cap, replacing the tubes inside the reservoir.
- Reattach the top of the protective cover.
- Let the reservoir liquid degas for 20 min. You should see noble gas bubbling through the water during this period.
- Close the system by opening the stopcock on the noble gas input line and closing the vent stopcock.

E. Add Water to the Humidifier Reservoir

- Unplug the hose adapter from the top of the humidifier reservoir (Figure 16).



Figure 16. Unplugging the hose adapter from the humidifier reservoir.

2. Fill the reservoir with deionized water (Figure 17). The photo on the right shows the filled reservoir.



Figure 17. Filling the reservoir with deionized water.

3. Close the cap securely and place the reservoir back onto the humidifier base unit (Figure 18).

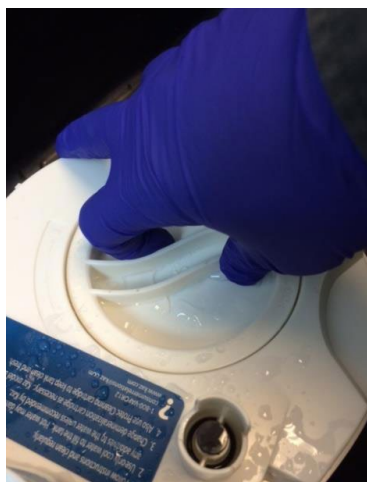


Figure 18. Closing the Reservoir.

4. Replace the hose adapter.

F. Run the Daily Warmup



IMPORTANT: Run the daily warmup each day prior to performing any experiments. Failure to do so will result in poor dispensing.

This procedure takes approximately 7 to 8 min.

1. Click the *Run* tab in the SmartChip Dispenser Software.

2. Click the [Daily Warmup] button in the **Instrument preparation** section of the *Startup* tab (Figure 19). The SmartChip MSND will do the following:
 - a. Display a dialog in the software indicating that the system is being brought up to pressure.
 - b. Send the head to the Purge position on the SmartChip MSND platform.
 - c. Prime the syringe path once.
 - d. Purge the syringe valves to remove any air that may be trapped in the syringe valves.



Figure 19. [Daily Warmup] button in the Instrument preparation section.

3. During the daily warmup, monitor the syringes in the fluidic module for trapped bubbles (Figure 20).

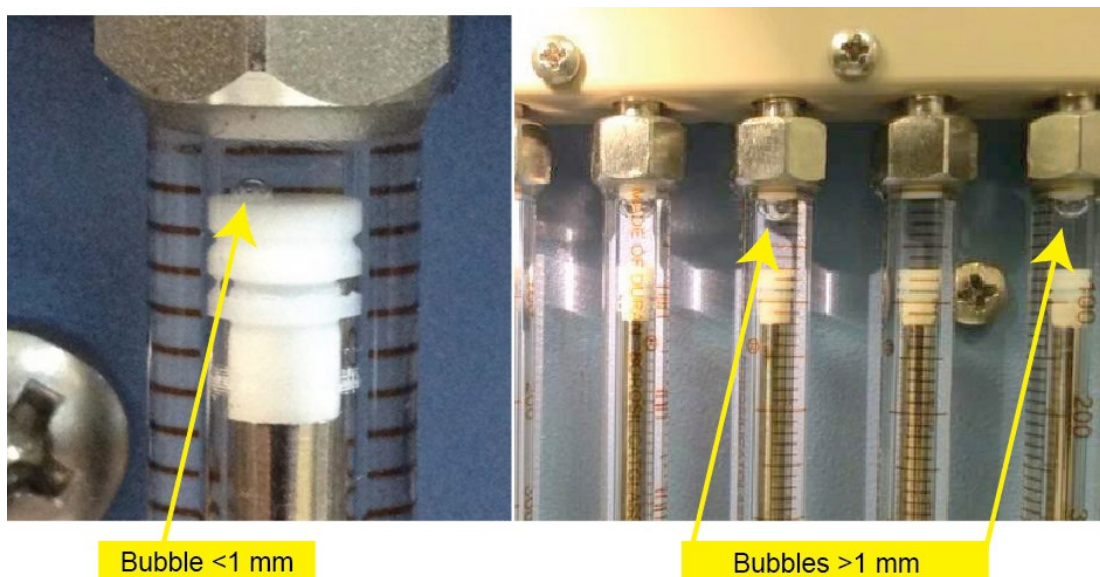


Figure 20. Monitoring the fluidic module for trapped bubbles. The bubble on the left is an acceptable size, while the bubbles on the right are too large.

Small bubbles are acceptable, but larger bubbles are not. If bubbles larger than 1 mm are observed:

- a. Allow the daily warmup procedure to finish.
- b. Repeat the first portion of the daily warmup procedure.
 - i. Click the [Daily Warmup] button.
 - ii. When the **Elapsed time** is 55 sec, click the [STOP] button (Figure 21).



Figure 21. *Daily Warmup* runtime dialog box.

- iii. If bubbles persist, repeat Step b above until all bubbles larger than 1 mm are purged from the syringe bank.

NOTE: If large bubbles are still present after three daily warmup cycles, we recommend an isopropyl alcohol wash. Refer to Section IX.F ("Maintenance: Remove Persistent Air Bubbles via Alcohol Wash").

G. Run the Tip Clean Procedure

The cleaning process takes about two minutes.

1. Click the *Advanced* tab in the SmartChip Dispenser Software.
2. Click the [Tip Clean] button in the **Manual Control** section (Figure 22).

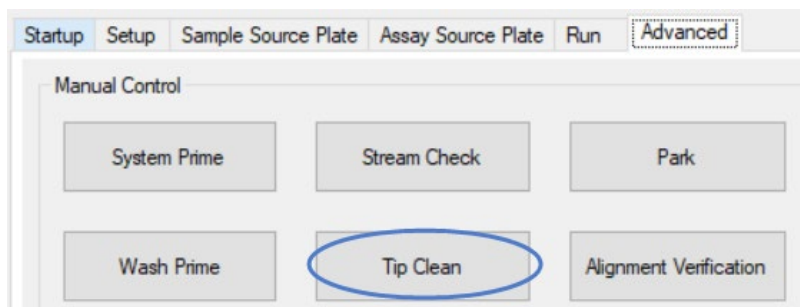


Figure 22. The [Tip Clean] button in the *Manual Control* section.

NOTE: The other buttons on the *Advanced* tab located under the buttons shown in Figure 22 are reserved for use by a certified Field Service Engineer. Customers are discouraged from using these.

VI. Protocol: Prepare the Source Plates

A source plate is a 384-well plate containing either the samples (i.e., a sample source plate) or the PCR assays (i.e., an assay source plate) that are to be dispensed using the SmartChip MSND.



IMPORTANT: Only nontreated NUNC Polypropylene 384-Well Plates (Takara Bio Cat. No. 430-000044-3) are validated for use on the SmartChip MSND.

This section has instructions for preparing source plates for the following applications or SmartChip type:

- Expression or genotyping analysis using SmartChip MyDesign Chips
- Expression or genotyping analysis using predispensed SmartChip Panels



IMPORTANT: Avoid introducing dust and debris to solutions that will be dispensed with the SmartChip MSND. They can cause the tips to clog.

Observe the following precautions when assembling sample and assay source plates:

- Consider assembling source plates in a dead air box to reduce environmental dust
- Wipe down the lab bench every day and wear gloves and a clean lab coat
- Use plates, tips, and tubes from new or carefully covered containers
- Work quickly and cover plates/tubes to minimize exposure to dust in the air

A. Prepare Source Plates for SmartChip MyDesign Chips

1. Prepare your samples and assays using the [SmartChip MyDesign Kit User Manual](#).
2. Pipette the following material into a 384-well plate based on the type of experiment you will be running:
 - For gene expression analysis: sample/PCR reagent mixtures containing cDNA, DNA
 - For genotyping: sample or sample/PCR reagent mixture containing DNA
 - Assays (on a separate source plate)

To make it easier to manually pipette into the 384-well source plates, we suggest implementing one of the following:

- Use the SmartChip Plate Layout Guides provided in the SmartChip MyDesign User Manual. Place the guide in the plate lid, under your source plate.
- Print the relevant source plate map(s) from Appendix B, Section C and refer to the printout at the bench.
- See the *Sample Source Plate* and *Assay Source Plate* tabs in the SmartChip Dispenser Software.

Tables 8 and 9 below shows recommended volumes per well and the number of wells in your sample source plate depending on the well volume of the chip.

Table 9. 384-well plate preparation for a 150 nl MyDesign chip: recommended volumes per well and number of wells for samples and assays.

SmartChip layout		Recommended volume and # of wells in source plate			
# of assays	# of samples	Sample source plate (volume/well)	# of wells per sample	Assay source plate (volume/well)	# of wells per assay
6	768	11.7 µl	1	17.9 µl	8
12	384	11.7 µl	1	17.9 µl	4
24	216	12.4 µl	1	17.9 µl	2
36	144	13.2 µl	1	20.3 µl	1
48	108	14.0 µl	1	17.9 µl	1
54	96	14.4 µl	1	17.1 µl	1
72	72	15.6 µl	1	15.6 µl	1
80	64	16.1 µl	1	15.1 µl	1
96	54	17.1 µl	1	14.4 µl	1
120	42	18.9 µl	1	13.7 µl	1
144	36	20.3 µl	1	13.2 µl	1
216	24	17.9 µl	2	12.4 µl	1
248	20	19.4 µl	2	12.2 µl	1
296	16	16.1 µl	4	12.0 µl	1
384	12	17.9 µl	4	11.7 µl	1

Table 10. 384-well plate preparation for a 250 nl MyDesign chip: recommended volumes per well and number of wells for samples and assays.

SmartChip layout		Recommended volume and # of wells in source plate			
# of assays	# of samples	Sample source plate (volume/well)	# of wells per sample	Assay source plate (volume/well)	# of wells per assay
6	768	12.3 µl	1	21.6 µl	8
12	384	12.3 µl	1	21.6 µl	4
24	216	13.6 µl	1	22.9 µl	2
36	144	15.0 µl	1	26.8 µl	1
48	108	16.1 µl	1	22.9 µl	1
54	96	16.9 µl	1	21.2 µl	1
72	72	18.9 µl	1	18.9 µl	1
80	64	19.8 µl	1	18.0 µl	1
96	54	21.2 µl	1	16.9 µl	1
120	42	20.9 µl	1	15.3 µl	1
144	36	26.8 µl	1	15.0 µl	1
216	24	22.9 µl	2	13.6 µl	1
248	20	24.6 µl	2	13.2 µl	1
296	16	19.1 µl	4	12.7 µl	1
384	12	21.6 µl	4	12.3 µl	1

- Pipette your assay/PCR reagent mixtures into a 384-well assay source plate.

NOTE: For SmartChip MyDesign Chips, the system is set up to include a single replicate of each reaction. To run replicates, use the same sample or assay/PCR reagent mixture for more than one sample or assay indicated in the source plate guides.

- After filling, seal the plate(s) with the adhesive film from the MSND 384-Well Source Plate and Seals and centrifuge at 3,220g for 5 min at room temperature.

IMPORTANT: The 384-Well Source Plate Seals included in MSND 384-Well Source Plate and Seals should be used for this. Please do not substitute with other sealing films.

B. Prepare Source Plates for Predispensed SmartChip Panels

- Prepare your samples and assays using the protocol provided with your SmartChip Custom Panels.
- Pipette the following mixture into a 384-well plate based on the type of experiment you will be running:

- For gene expression analysis: SmartChip TB Green Gene Expression Master Mix/your cDNA
- For genotyping: SmartChip Probe qPCR Master Mix/your DNA

To make it easier to manually pipette into the 384-well source plates:

- Use the provided SmartChip Plate Layout Guides. Place the guide in the plate lid, under your source plate.
- Print the relevant source plate map(s) from Appendix B, Section C to serve as a reference at the bench.
- Use the *Sample Source Plate* and *Assay Source Plate* tabs in the SmartChip Dispenser Software.

Tables 10 and 11 show recommended volumes per well and number of wells for sample source plates targeting predispensed SmartChip Panel chips.

Table 11. Sample source plates for gene expression analysis: predispensed SmartChip Panels.

SmartChip layout		Minimum–recommended volume/well, # of wells	Total sample volume	
# of assays	# of samples		Minimum (µl)	Recommended (µl)
12	96	15–18 µl per well, 1 well	15	18
24	48	21–25 µl per well, 1 well	21	25
48	24	21–25 µl per well, 2 wells	42	50
96	12	21–25 µl per well, 4 wells	84	100
192	6	23–27 µl per well, 7 wells	158	190
384	3	23–27 µl per well, 14 wells	316	379

Table 12. Sample source plates for SNP genotyping: predisposed SmartChip Panels.

SmartChip layout		Minimum–recommended volume/well, # of wells	Total Sample Volume	
# of assays	# of samples		Minimum (µl)	Recommended (µl)
12	384	10.5–12.6 µl per well, 1 well	10.5	12.6
24	216	11.6–14.0 µl per well, 1 well	11.6	14.0
48	108	14.3–17.1 µl per well, 1 well	14.3	17.1
72	72	16.9–20.3 µl per well, 1 well	16.9	20.3
96	54	19.6–23.5 µl per well, 1 well	19.6	23.5
120	42	22.6–27.1 µl per well, 1 well	22.6	27.1
192	24	20.9–25.1 µl per well, 2 wells	41.8	50.1
384	12	20.9–25.1 µl per well, 4 wells	83.5	100.2

NOTE: Use source plates immediately or store on ice and centrifuge just before use.

- After filling, seal plate(s) with adhesive film from MSND 384-Well Source Plate and Seals and centrifuge at 3,220g for 5 min at room temperature.

C. Prepare Source Plates Using Automation

If you plan to dispense from a 384-well source plate containing assays and/or samples filled by an automated pipette, please refer to Appendix B, Section C for best practices and sample plate maps.

VII. Protocol: Configure the SmartChip MultiSample NanoDispenser (MSND)

The SmartChip Dispenser Software controls all SmartChip MSND operations: dispensing your samples/assays into the nanowells of SmartChip MyDesign chips or panels and warming up and cleaning the instrument.

For real-time PCR applications, such as expression and genotyping analysis, SmartChip Dispenser Software uses information you provide about the chip contents and their locations on the chip to create the SmartChip Layout file that is needed to run the real-time PCRs on the SmartChip cycler. You can input detailed information such as your SmartChip type and number, the number of experimental samples, sample names, sample concentrations, and the PCR assays (if you are using a SmartChip MyDesign Chip).

A. Chip Type Selector: Specify the SmartChip Type Being Used

The software needs to be configured to match the chip that is used.

- Go into the **Utilities > Select chip type** menu option. The *Chip Type Selector* dialogue window will pop up.

2. Select for one of the two options in the dropdown menu:
 - For **150 nl** SmartChip MyDesign or predisensed SmartChip Panel chips, select '72 rows x 72 columns 1 zone non-SBS'—first option, highlighted in Figure 23 (below)
 - For **250 nl** SmartChip MyDesign chips, select '72 rows x 72 columns 1 zone non-SBS 250 nl'—second option, shown unhighlighted in the Figure 23 dropdown menu

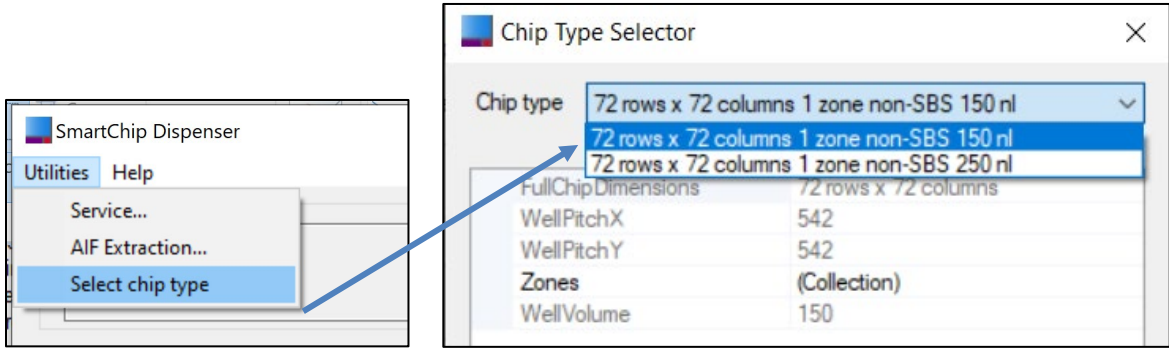


Figure 23. The Utilities > Select chip type workflow and Chip Type Selector dialog. The size of the chip (150 nl or 250 nl) is selected in the "Chip Type" dropdown menu.

Note that the Main GUI has an indicator showing which chip type is currently selected:



Figure 24. Finding the selected chip well volume. After selecting the size of the chip (Figure 23), the related volume will display on the main UI. Top: 150 nl. Bottom: 250 nl.

B. Setup Tab: Enter Information About Your Experiment

1. Click the *Setup* tab (Figure 25).

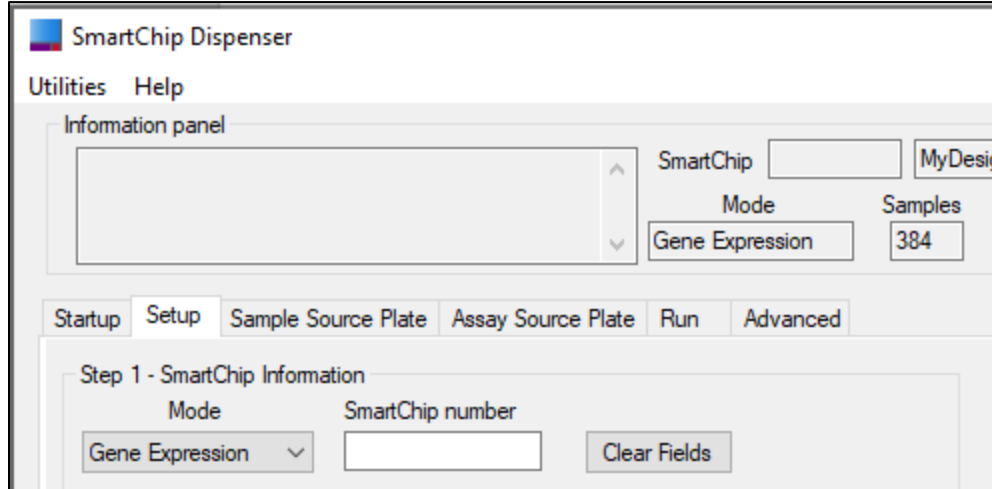


Figure 25. *Setup* tab in the SmartChip Dispenser Software.

2. Enter information about the chip as described below.
 - a. Select the type of experiment from the "Mode" dropdown menu (Figure 26).
 - For microRNA analysis, select 'Gene Expression'
 - For genotyping analysis, select 'Genotyping'

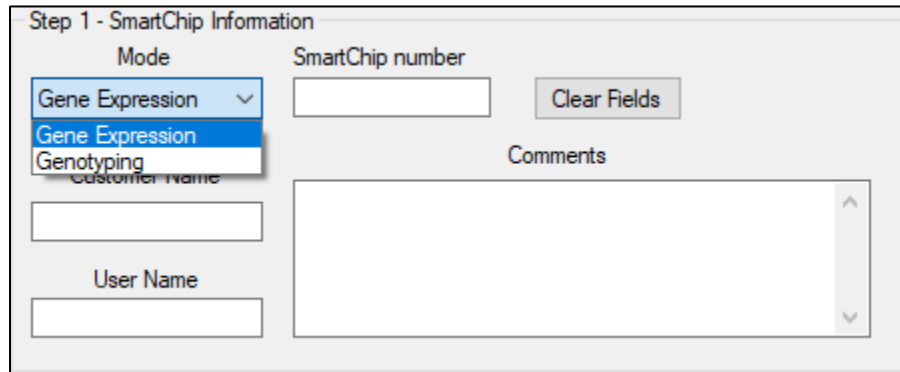


Figure 26. Mode list.

- b. (Optional, but highly recommended for real-time PCR applications): Enter a value into the "SmartChip number". You can either type the number in *or* place your cursor in the "SmartChip number" field and use the barcode reader to scan the 2-D barcode on the back of the chip.

The SmartChip number can be used later to identify the SmartChip Layout file for this chip.
 - c. (Optional) Enter relevant information in the "Customer Name", "User Name", and "Comments" fields.

3. Select the "SmartChip Format" in the **Step 2—Dispense Options** section (Figure 27).
 - Select the 'Predispensed' radio button if you are using a SmartChip Panel chip. The "Dispense Volume" field will automatically display '100 nl' for this selection.

NOTE: If a 250 nl chip type was specified, the 'Predispensed' option will be grayed out as in Figure 25, below).

- Select the 'MyDesign' radio button if you are using a MyDesign Chip.
 - If you are using a 150 nl chip, the "Dispense Volume" field displays '50 nl' corresponding to 50 nl of sample/PCR reagent mixture then 50 nl of assay/PCR reagent mixtures.



Figure 27. SmartChip dispense options for a 150 nl chip.

- If you are using a 250 nl chip, the "Dispense Volume" field displays '100 nl', corresponding to 100 nl of sample/PCR reagent mixture then 100 nl of assay/PCR reagent mixtures.



Figure 28. SmartChip dispense options for a 250 nl MyDesign chip.

4. Select the "SmartChip Layout" (Figure 29) in the **Step 3—SmartChip Layout** dropdown menu.

The option selection should be the desired configuration for your experimental setup (number of assays and number of samples). Refer to Section VI, "Prepare the Source Plates" for more information.

Step 3 - SmartChip Layout		
80 assays	64 samples	1 replicate
6 assays	768 samples	1 replicate
12 assays	384 samples	1 replicate
24 assays	216 samples	1 replicate
36 assays	144 samples	1 replicate
48 assays	108 samples	1 replicate
54 assays	96 samples	1 replicate
72 assays	72 samples	1 replicate
80 assays	64 samples	1 replicate
96 assays	54 samples	1 replicate
120 assays	42 samples	1 replicate
144 assays	36 samples	1 replicate
216 assays	24 samples	1 replicate
248 assays	20 samples	1 replicate
296 assays	16 samples	1 replicate
384 assays	12 samples	1 replicate

Figure 29. SmartChip assays X samples layout options.

C. Sample Source Plate Tab: Enter Your Sample Information

1. Click the *Sample Source Plate* tab (Figure 30). A sample source plate map that corresponds to the SmartChip Layout (selected on the *Setup* tab in the previous step) is shown. You can use this map as a guide for placing sample mixtures into your sample source plate or use the printable 384-well source plate maps in Appendix C.

NOTE: For the 6 assay and 768 samples dispense pattern, users will need to select the radio buttons for "Plate 1" and "Plate 2" (highlighted by the red box in Figure 30) to see all 768 samples in the source plate map grid.

Startup Setup **Sample Source Plate** Assay Source Plate Run Advanced

Barcode Plate 1 Plate 2

Samples containing "pos" in their name will be highlighted in green.
Samples containing "neg" or "ntc" in their name will be red.

A	S385	S401	S417	S433	S449	S465	S481	S497	S513	S529	S545	S561	S577	S593	S609	S625	S641	S657	S673	S689	S705	S721	S737	S753
B	S386	S402	S418	S434	S450	S466	S482	S498	S514	S530	S546	S562	S578	S594	S610	S626	S642	S658	S674	S690	S706	S722	S738	S754
C	S387	S403	S419	S435	S451	S467	S483	S499	S515	S531	S547	S563	S579	S595	S611	S627	S643	S659	S675	S691	S707	S723	S739	S755
D	S388	S404	S420	S436	S452	S468	S484	S500	S516	S532	S548	S564	S580	S596	S612	S628	S644	S660	S676	S692	S708	S724	S740	S756
E	S389	S405	S421	S437	S453	S469	S485	S501	S517	S533	S549	S565	S581	S597	S613	S629	S645	S661	S677	S693	S709	S725	S741	S757
F	S390	S406	S422	S438	S454	S470	S486	S502	S518	S534	S550	S566	S582	S598	S614	S630	S646	S662	S678	S694	S710	S726	S742	S758
G	S391	S407	S423	S439	S455	S471	S487	S503	S519	S535	S551	S567	S583	S599	S615	S631	S647	S663	S679	S695	S711	S727	S743	S759
H	S392	S408	S424	S440	S456	S472	S488	S504	S520	S536	S552	S568	S584	S600	S616	S632	S648	S664	S680	S696	S712	S728	S744	S760
I	S393	S409	S425	S441	S457	S473	S489	S505	S521	S537	S553	S569	S585	S601	S617	S633	S649	S665	S681	S697	S713	S729	S745	S761
J	S394	S410	S426	S442	S458	S474	S490	S506	S522	S538	S554	S570	S586	S602	S618	S634	S650	S666	S682	S698	S714	S730	S746	S762
K	S395	S411	S427	S443	S459	S475	S491	S507	S523	S539	S555	S571	S587	S603	S619	S635	S651	S667	S683	S699	S715	S731	S747	S763
L	S396	S412	S428	S444	S460	S476	S492	S508	S524	S540	S556	S572	S588	S604	S620	S636	S652	S668	S684	S700	S716	S732	S748	S764
M	S397	S413	S429	S445	S461	S477	S493	S509	S525	S541	S557	S573	S589	S605	S621	S637	S653	S669	S685	S701	S717	S733	S749	S765
N	S398	S414	S430	S446	S462	S478	S494	S510	S526	S542	S558	S574	S590	S606	S622	S638	S654	S670	S686	S702	S718	S734	S750	S766
O	S399	S415	S431	S447	S463	S479	S495	S511	S527	S543	S559	S575	S591	S607	S623	S639	S655	S671	S687	S703	S719	S735	S751	S767
P	S400	S416	S432	S448	S464	S480	S496	S512	S528	S544	S560	S576	S592	S608	S624	S640	S656	S672	S688	S704	S720	S736	S752	S768

Step 4 - Sample Source Plate Enter sample information in plate map above or open existing sample source plate file

Selected Sample Source Plate

Sample View
Name

Figure 30. Sample source plate tab.

2. Add information about the samples in the sample source plate grid, using one of the methods below:
 - a. Load a sample source plate file (Figure 31).

If you have a file describing the location of samples in your source plate:

- i. Select [Import Sample Source Plate File...]
- ii. Navigate to the file location
- iii. Select the file by mouse-clicking on the file name
- iv. Click [Open]

Step 4 - Sample Source Plate Enter sample information in plate map above or open existing sample source plate file

Selected Sample Source Plate

Figure 31. Loading a sample source plate file.

- b. Manually enter sample information.
 - i. Select the sample attribute from the "Sample View" list (Figure 32). The attributes listed depend on the selection made in the "Mode" dropdown in the *Setup* tab (Figure 26).

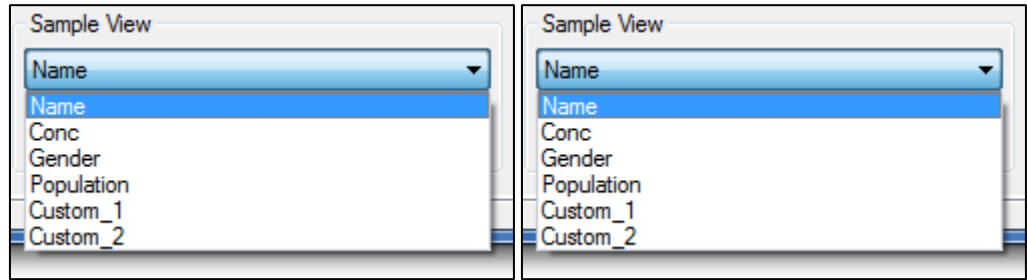


Figure 32. Sample View list.

- ii. Enter information for the selected attribute into the sample source plate grid. Place your cursor in the cell you want to edit and type the values or copy and paste from Excel.
- 3. Click the "Barcode" field and then scan the barcode on the sample source plate.
- 4. Click the [Save Source Plate File] button. You can reuse this sample source plate file in subsequent experiments if desired.

Additional options when working with the sample source plate grid

NOTE: The functions described below are also available in the assay source plate grid.

- 1. Right-click a cell to copy the contents of the cell.
- 2. After copying, left-click a cell or a range of cells to paste the content.
- 3. Hold the mouse over the cell to see all the information entered about the well (Figure 33).




Figure 33. Well information.

- 4. Double-click the border of the column header to expand the column wide enough to view the contents (Figure 34).

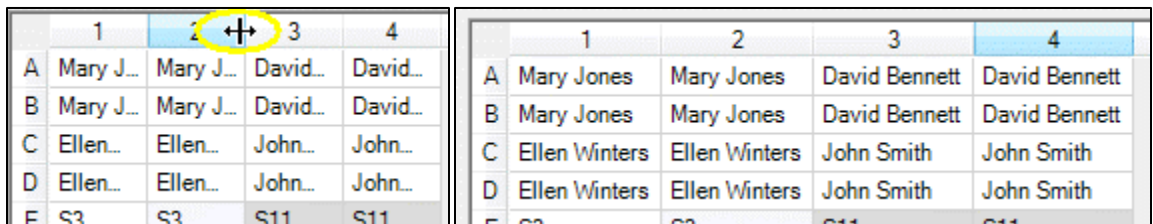


Figure 34. Increasing the width of a source plate grid column in MS Excel.

D. Assay Source Plate Tab: Enter PCR Assay Information (MyDesign Chips Only)

NOTE: The assay source plate file created in this section can be reused in subsequent chip runs or experiments with identical assay parameters, if desired.

1. Click the *Assay Source Plate* tab (Figure 35). An assay source plate map that corresponds to the SmartChip Layout (selected on the *Setup* tab) is shown. You can use this map as a guide for placing assay mixtures into your assay source plate or the printable 384-well source plate maps in Appendix B, Section D.

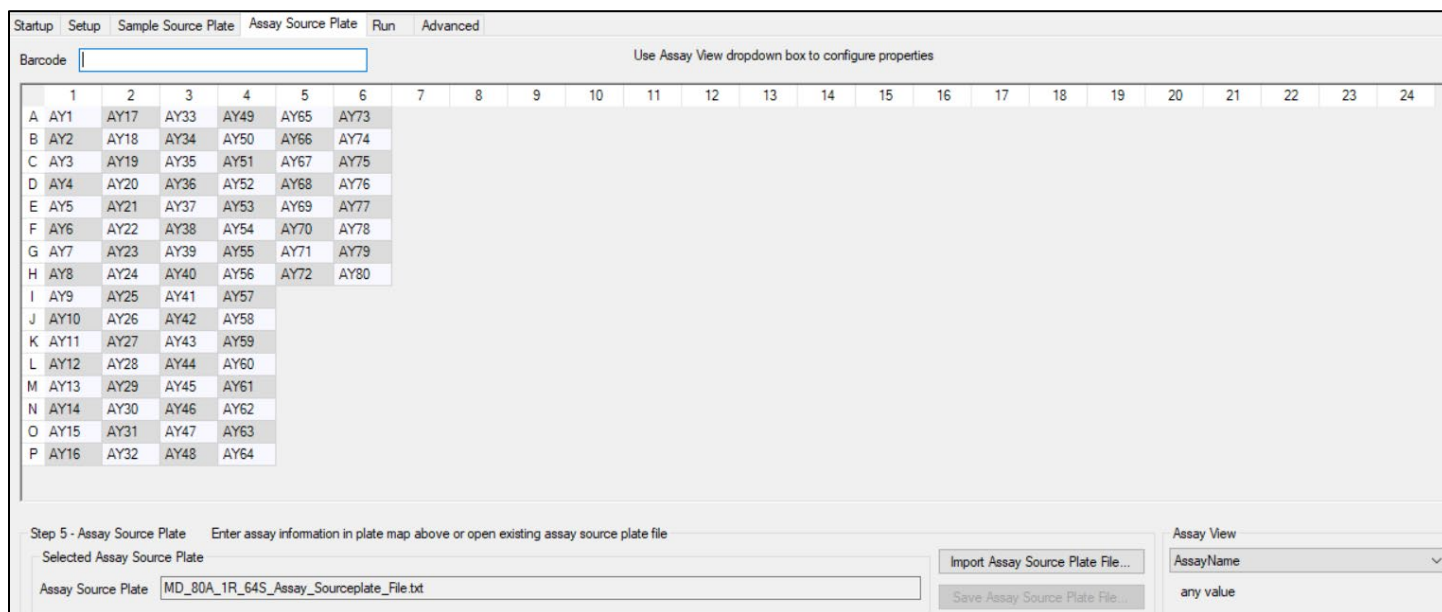


Figure 35. Assay source plate tab.

1. Enter information about the PCR assays in the assay source plate grid, using one of the methods below:
 - a. Load an assay source plate file (Figure 36)

If you have a file describing the location of samples in your source plate:

- i. Select [Import Assay Source Plate File...]
- ii. Navigate to the file location
- iii. Select the file by mouse-clicking on the file name
- iv. Click [Open]

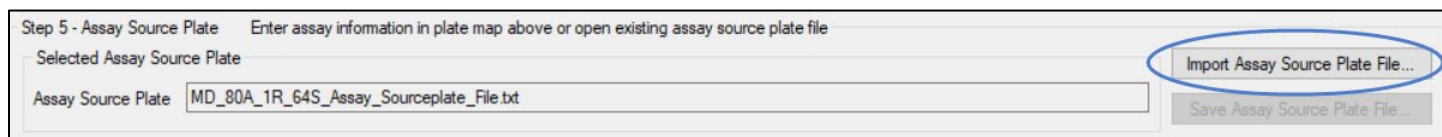


Figure 36. Loading an assay source plate file.

- b. Manually enter the assay information

- i. Select the assay attribute from the "Assay View" list (Figure 37).

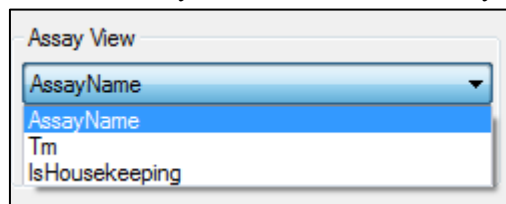


Figure 37. Assay View list.

- ii. Enter the information for the selected attribute into the assay source plate grid. Place your cursor in the cell you want to edit and type the values or copy and paste from Excel.
2. Click the "Barcode" field, and then scan the barcode on the assay source plate.
 3. Click the [Save Assay Source Plate File] button to save the file.

E. Generate and Save Your SmartChip Layout File

The SmartChip Layout file is needed by the qPCR software to run your sample and assays on the SmartChip cycler. The extension on the SmartChip Layout file indicates the type of information it contains:

- **<filename>.pd** : contains only sample information. For use with a predisposed SmartChip Panel.
- **<filename>.md**: contains sample and PCR assay information. For use with a SmartChip MyDesign Chip.

To create the SmartChip Layout File:

1. Click the [Generate SmartChip Layout File] button (Figure 38).

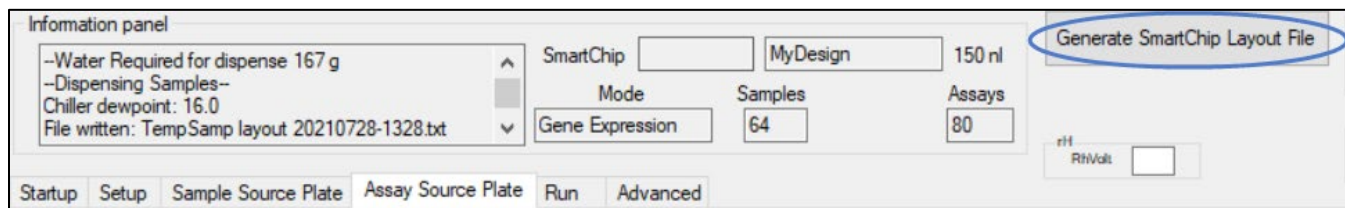


Figure 38. Generating a SmartChip Layout file.

2. Enter information in the *Save SmartChip Layout File* dialog as described below.
 - a. Edit the file name, if desired. The default name includes the SmartChip number, the date, and the time.
 - b. Choose a location to save the file.

This file is needed to run your reactions on the SmartChip cycler, so you may want to save it to a USB memory stick or a network folder. If you do not specify a location for the file, the default location is:

C:\ProgramData\takara\SmartChipDispenser

VIII. Protocol: Dispense Using the SmartChip MSND

NOTE: You will be cleaning the SmartChip MSND periodically during this protocol as described below.

- After each dispense:
 1. Remove the 384-well plate from the plate nest and properly dispose of it
 2. Inspect the dispensing platform for any debris and wipe down with 70% isopropanol
- After the final dispense of the day:
 1. Perform the 'after each dispense' protocol above
 2. Perform the tip clean procedure described in Section V.G ("Run the Tip Clean Procedure")

A. Place the Nanowell Chip in the SmartChip MSND

1. Remove the protective film from your SmartChip Panel or MyDesign Chip.
If dispensing assays (second dispense) into a MyDesign chip, carefully remove the intermediate film.
2. Visually inspect the dispensing platform and clean it if there is any debris.
3. Place the chip on the platform inside the stage module, as described below (Figure 39).
 - a. Stretch the arms of the clip apart and angle the chip onto the dispensing platform, with the beveled corner on the lower right and the edges of the chip pressed against the three alignment pins.
 - b. Carefully release the clip that holds the chip in position.

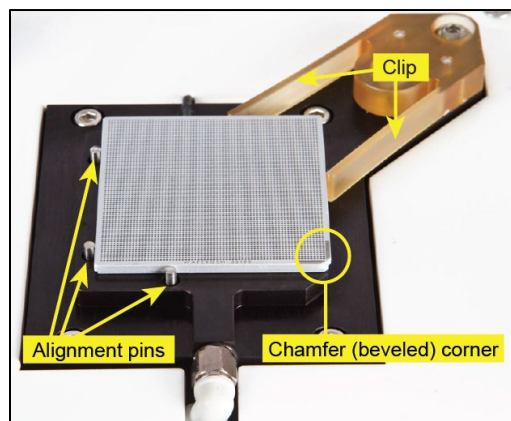


Figure 39. Placing the chip on the dispensing platform inside the stage module.

B. Place the Source Plate in the SmartChip MSND

1. If you haven't already done so, centrifuge the source plate at 3,220g for 5 min at 20–25°C.
2. Remove the MSND 384-Well Source Plate and Seals adhesive film.

3. Place the 384-well source plate on the plate nest with the A1 position in the top, back right corner, as shown in Figure 40.

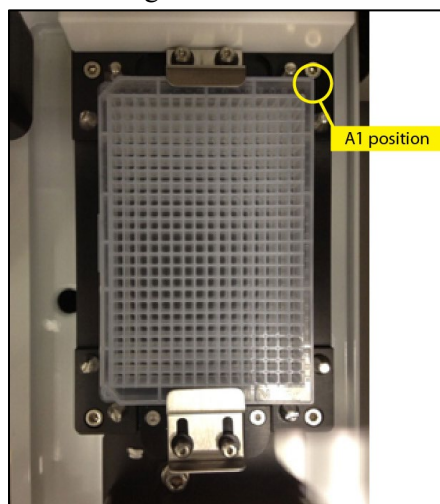


Figure 40. Sample source plate on the plate nest.

4. Close the environmental chamber doors.

C. Dispense into the Nanowell Chip

The following section can be used to dispense either samples, sample/PCR reagent mixture, or assays/PCR reagent mixture into a SmartChip MyDesign or SmartChip Panel predisposed chip.

NOTES

- **Section 1**, below, covers the default dispense process for samples and assays
- If dispensing samples in a 6 assay X 768 sample layout, refer to Appendix B.B, "Workflow Guidelines for 768-Sample Dispense"
- If you need to dispense out of order, refer to **Section 2** (VIII.C.2)



IMPORTANT OPERATIONAL NOTES

- Do not open the door of the stage module while the SmartChip MSND is dispensing. If the door is open, the chip can become contaminated. Additionally, when the door is open, evaporation from the nanowells can occur, resulting in changes to concentrations of the reagents in the chip.
- Do not touch the barcode reader while the SmartChip MSND is dispensing. Operating the reader while the system is dispensing could interfere with the instrument run.

1. Default dispense process for samples and assays

Click the *Run* tab in the SmartChip Dispenser Software and then click [Dispense Samples] if you are dispensing from your Sample plate, or [Dispense Assays] if you are dispensing from your Assay source plate (Figure 41).

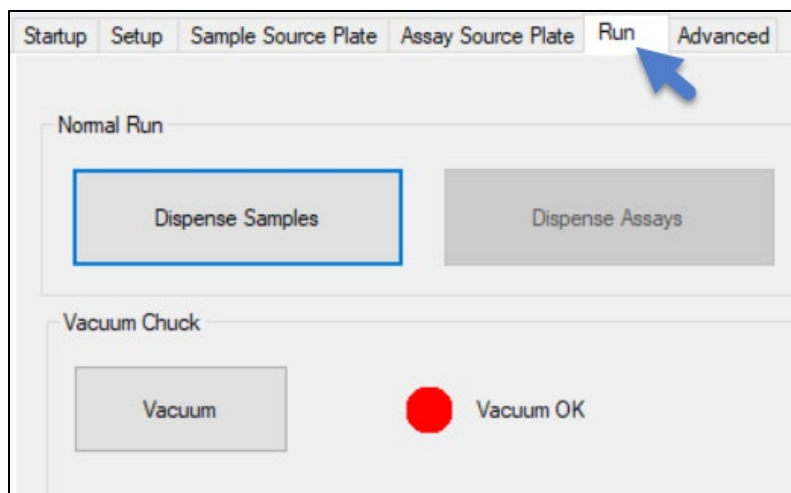


Figure 41. *Run* tab.

NOTE: For some SmartChip instruments, the scale for the source bottle turns off after a period of inactivity. If a *Check Water Level* warning message similar to Figure 42 (below) displays, it means that this has occurred.

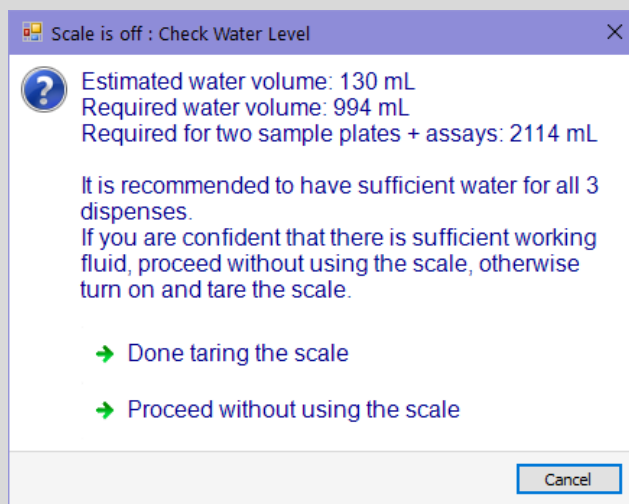


Figure 42. *Check Water Level* pop-up error message.

If this message is seen:

- a. Remove the source bottle from the scale
- b. Turn on the scale and make sure it has been tared
- c. Place the source bottle back on the scale
- d. Click the text in the error window [Done taring the scale]

If the humidity is not high enough, the [Dispense Samples] button flashes and a message appears (Figure 43). When the humidity reaches the correct level, the run will begin automatically.

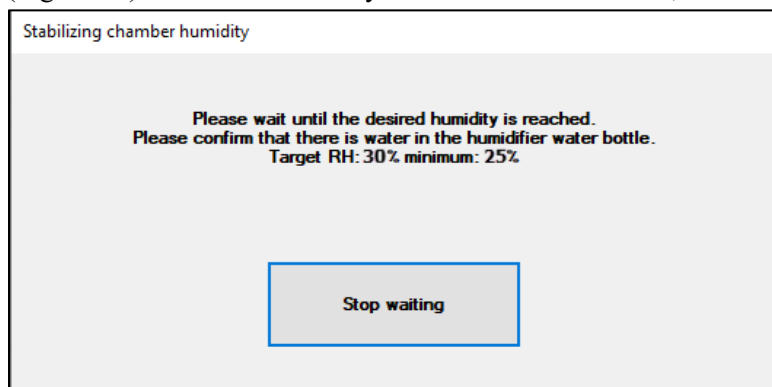


Figure 43. Pop-up displayed when the system is adjusting the humidity of the environmental chamber prior to dispense.

If the [Stop waiting] button is clicked while the unit is trying to reach minimum humidity, users have three options to choose from (Figure 44).

NOTE: We strongly recommend customers wait until minimum humidity is reached.

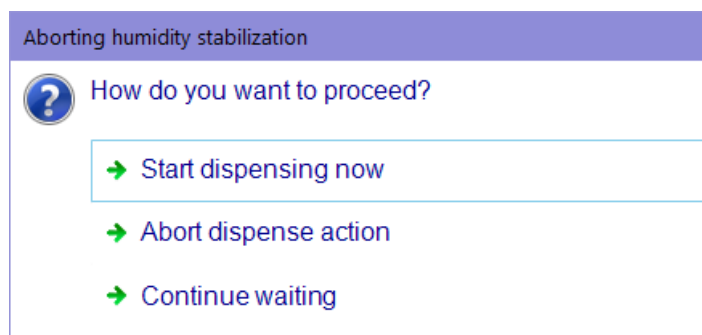


Figure 44. Pop-up displayed when customer selects [Stop Waiting] in the pop-up shown in Figure 43.

If the system times out while equilibrating the chamber to minimum humidity, a pop-up message will prompt you to either start the dispense or abort (first two options in Figure 44). If you proceed with the dispense in this situation, you may experience an adverse impact on your experiment. Please contact [technical support](#) for guidance.

2. How to enable an unordered dispense

By default, the workflow allows access to one dispense at a time to facilitate the recommended application (Figure 45, next page).

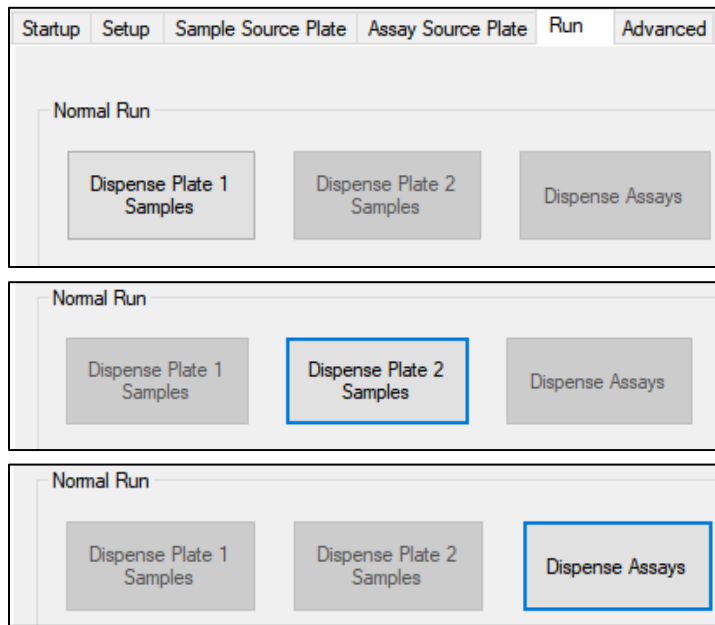


Figure 45. Dispense button behavior in the *Run* tab for the default (ordered) dispense. Buttons are displayed as active (black font) only in stepwise sequence. Inactive buttons (gray font) cannot be clicked out of order.

If needed, the default, ordered dispense mode can be disabled by going into the *Advanced* tab and checking the box next to "Allow Unordered Dispense".

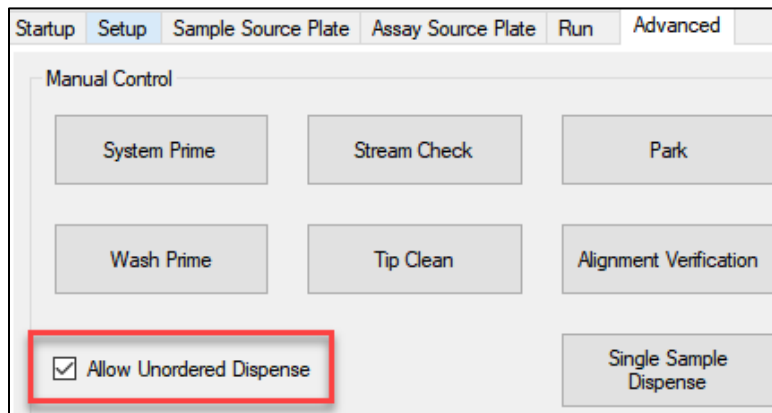


Figure 46. Where to find the "Allow Unordered Dispense" check box in the *Advanced* tab.

When checked, all dispense buttons under the *Run* tab are active and can be clicked, in any order.

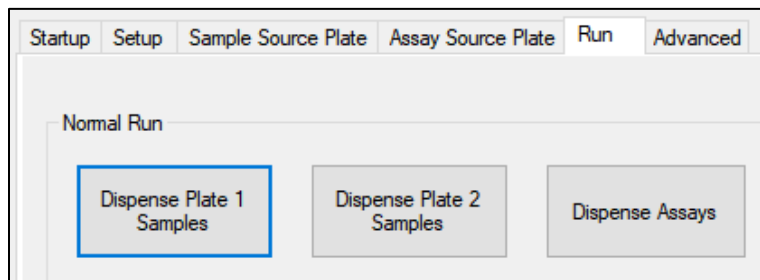


Figure 47. Dispense button behavior in the *Run* tab for an unordered dispense. All buttons are active (black font).

To revert back to the ordered dispense mode, uncheck the "Allow Unordered Dispense" box.

D. Blot, Seal, and Spin the Chip

1. After dispensing is complete, promptly blot the chip for 2 sec.
 - a. Place the chip, wells facing up, on a clean lab wipe.
 - b. Gently place a piece of SmartChip blotting paper directly on top of the chip. Make sure that the blotting paper covers the entire face of the chip.
 - c. Pick up the SmartChip Blotter by the top handle and place the flat face of the blotter against the blotting paper on the chip. The blotter should extend beyond the edges of the chip.
 - d. Let the blotter rest on top of the blotting paper for exactly 2 sec without pressing down—the weight of the blotter is sufficient for adequate blotting.
 - e. Remove the blotter, and then gently remove the blotting paper and dispose of it in a biohazard container.
2. Quickly seal the loaded chip with the appropriate film.

Table 13. Selecting the correct sealing film to use on the nanowell chip for each SmartChip type.

Chip type	Dispense type	Film type
Predispensed SmartChip Panel	Sample dispense	SmartChip cycling film*
MyDesign chip	Sample dispense	SmartChip Intermediate Film†
	Assay dispense	Cycler Sealing and Pressure Film*†

*SmartChip Cycling Film and Cycler Sealing and Pressure Film are the same product under different names; both look like the film shown in Figures 45 and 46, below.

†Film is included in the SmartChip MyDesign Kit.

The steps below illustrate application of the SmartChip cycling film and Cycler Sealing and Pressure Film.

NOTE: Other than how the backing is peeled from the film, application of the intermediate film will be performed similarly.

- a. Remove the backing from the adhesive film.
 With cycling film, remove the backing only from the center of the film (Figure 48). Leave the blue backing around the periphery of the film in place.

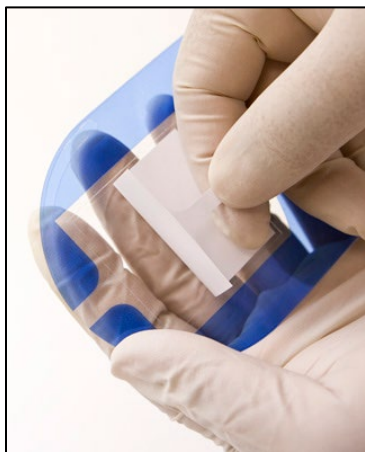


Figure 48. Removing the backing from the SmartChip cycling film.

- b. Center the square adhesive portion of the film over the chip and press into place. The film must cover the chip entirely but does not need to align perfectly.

For cycling film, place the film in the orientation shown below (Figure 49).

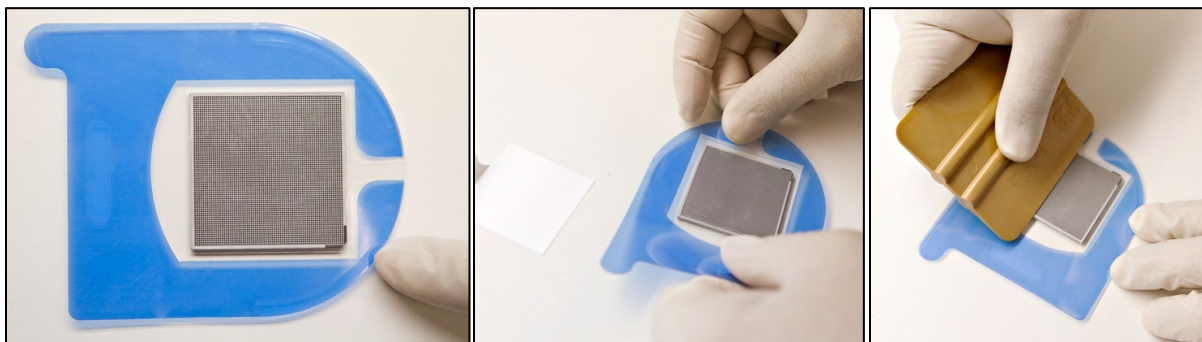


Figure 49. Placing the cycling film on the chip.



IMPORTANT: Be sure to place the cycling film on the chip in the orientation shown in the photos above. In the photo on the left, in Figure 49, the chamfered corner of the chip is at the bottom right in the photo; our scientist is pointing to it.

- c. Use your fingers to press and smooth the seal, starting at the center of the chip and moving toward the edges.
- d. To make sure that a strong seal is achieved, apply pressure with the seal applicator from the center of the chip outward. Repeat 8 times, rotating the chip 45 degrees each time to seal all edges and corners.

NOTE: Small bubbles on the periphery of the chip will not cause problems, but bubbles on top of the nanowells may interfere with gathering information on the wells under the bubbles. It is recommended to continue the procedure, as it will only affect a small area of the chip. Do NOT try to remove and reapply the film to correct it—this will likely cause cross-contamination between wells.

3. Using the chip spinner, centrifuge the chip at 3,220g for 5 minutes at 4°C as described below.
 - a. Place your chip(s) in the Chip Spinner(s).
 - b. Counterbalance with either a second chip spinner and chip or with the balance plate (Figure 50).

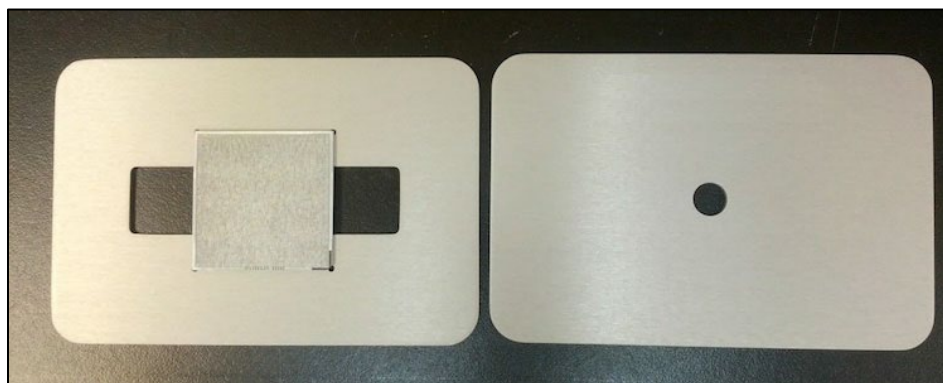


Figure 50. Chip spinner and plate (left) and balance plate (right).

- Determine the next step of the protocol by following the definitions in Table 14.

Table 14. Determining the next step of the protocol after MSND dispense.

Chip type	Dispense type	Next step
SmartChip Panel	Sample dispense	Run your PCRs on the SmartChip cycler*
MyDesign chip	Sample dispense	Clean the MSND and repeat Sections VIII.A–D for assay dispense†
	Assay dispense	Run your PCRs on the SmartChip cycler*

*Refer to the [SmartChip Real-Time PCR System / SmartChip qPCR Software User Manual](#)

†Dispensed MyDesign chips can optionally be stored for up to 4 hr at 4°C. After storage and immediately prior to use, allow sealed chips to warm to room temperature, and then spin for 5 min at 3,220g.

E. Run PCRs on the SmartChip Cycler

See the [SmartChip Real-Time PCR System / SmartChip qPCR Software User Manual](#) for complete instructions on thermal cycling the filled SmartChip Panel or MyDesign chip.

F. Clean the MSND

After starting the PCRs on the SmartChip cycler, return to the MSND to perform the appropriate cleaning procedure as described in the note at the beginning of Section VIII.

IX. Maintenance



CAUTION: There are no user-serviceable parts inside the instrument. Service of internal parts should be performed by a qualified Takara Bio service technician.

A. Daily Maintenance

Daily Maintenance procedures help ensure optimal instrument operation and prevent problems. They are described in "Protocol: Prepare the SmartChip MultiSample NanoDispenser (MSND)" (Section V).

B. Shutdown Procedure

Follow these instructions to completely shut down the SmartChip MSND if the instrument will not be used for more than a week.

If the SmartChip MSND will not be in use for 1–4 weeks

Please follow the steps below:

- Leave the instrument and the computer turned on. The software will automatically run the daily warmup (Section V.F) after being idle for ~24 hours.
- Check the pressure reservoir every ~2 weeks. Fill and degas, as needed (Section V.D).

If the SmartChip MSND will be idle for more than four weeks

Please follow the steps below to do a complete shutdown the system:

- Park the system by pressing the [Park] button in the *Run* tab of the software.
- Visually inspect the dispensing platform for any debris and wipe down with 70% isopropanol.
- Perform the tip clean procedure (Section V.G).
- Shut down the MSND + GUI.

5. Turn off the laptop.
6. Turn off the pump box (the rectangular box where the computer sits). There is a switch on the bottom left-hand side, located on the back of the pump box.
7. Turn off the fluidic module. There is a switch on the bottom left-hand side of the back of the fluidic module.

NOTE: Wait a few minutes for the system to reach setpoint before proceeding to the next step.

C. Restart the SmartChip MSND from a Complete Shutdown

Please follow the steps below to power up the system from a complete shutdown.

1. Turn on the fluidic module. There is a switch on the bottom left-hand side of the back of the fluidic module.
2. Turn on the pump box (the rectangular box where the computer sits). There is a switch on the bottom left-hand side, located on the back of the pump box.
3. Turn on the laptop.
4. Turn on the electronic scale, if off. Lift the pressure reservoir bottle to tare the scale.
5. Turn on the MSND + GUI.

NOTE: Wait a few minutes for the system to reach setpoint before proceeding to the next step.

6. Check the water in the reservoir, add water, and degas the water.
7. After 20 minutes of degassing, continue with a daily warmup (Section V.F).

D. Clean the Humidifier

Every 6 months, empty and clean the humidifier.

1. Rinse the humidifier chamber with a 1:10 dilution of commercial bleach (0.6% sodium hypochlorite).
2. Rinse 3 times with deionized, filtered water.
3. Let the humidifier dry.
4. Refill with deionized, filtered water.

E. Verify the Dispensing Tip Alignment

Around every 20 runs of the SmartChip MSND or approximately every two weeks, verify the alignment of the dispensing tip.

Procedure summary:

- The alignment verification run dispenses fluorescent Imitation Master Mix into the Nanodispenser Alignment Chip (Takara Bio, Cat. No. 640041, referred to below as "alignment chip") provided with the instrument
 - After dispensing, you will look at the alignment chip under UV light and magnification to check dispensing consistency
1. Prepare a source plate containing the Imitation Master Mix as described below.
 - a. Pipette 15.5 μ l of Imitation Master Mix with UV Dye & ROX (Takara Bio, Cat. No. 640026) into all of the wells in Columns 1 and 2 of a 384-well plate.
 - b. Put the plate into the plate nest, with the filled wells closer to the wash trough.

2. Seal the bottom of the SmartChip alignment chip with Nanodispenser Alignment Chip Film (Takara Bio, Cat. No. 640030, referred to as "alignment chip film"), as described below.
 - a. Hold the alignment chip film by the tab and pull it apart. Carefully peel off the backing completely.
 - b. With the bottom of the alignment chip facing up and the beveled corner in the lower left as you face the chip, apply the film to the back of the chip so that the tab is on the right side (Figure 51).

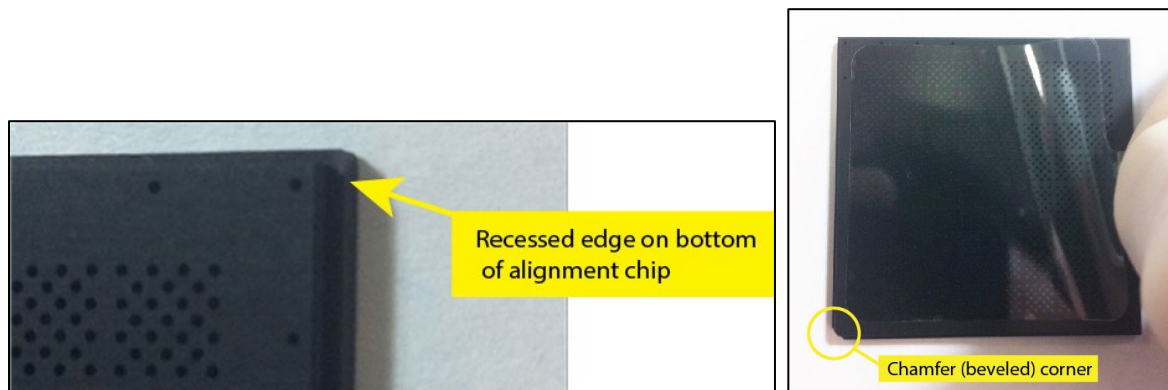


Figure 51. Sealing the alignment chip with alignment chip film.

- c. Remove any air trapped between the film and the alignment chip by pushing the bubbles toward the outer edges of the film.
3. Position the chip on the SmartChip MSND as described below.
 - a. Turn the chip over so that the film is on the bottom. Place the chip on the dispensing platform of the SmartChip MSND, with the chamfer (beveled corner) on the lower right. Be sure that the chip is flat, the chamfer is in the lower right corner, and the chip sits snugly against the three alignment posts (Figure 52).

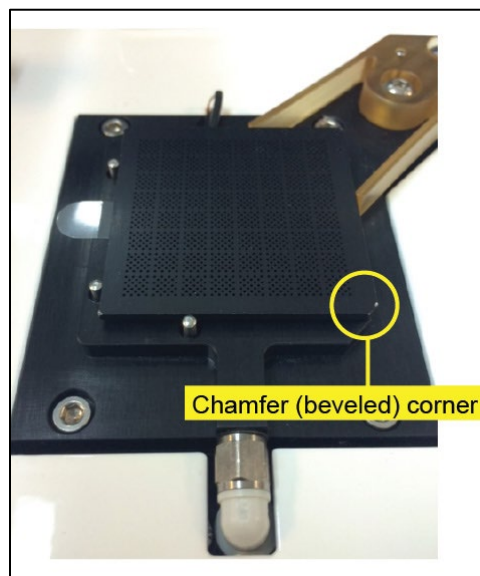


Figure 52. Positioning the sealed alignment chip on the SmartChip MSND.

- b. Close the front and side doors.

4. Perform the alignment verification using the SmartChip Dispenser Software. Click the *Advanced* tab and then click the [Alignment Verification] button (Figure 53) to start dispensing.

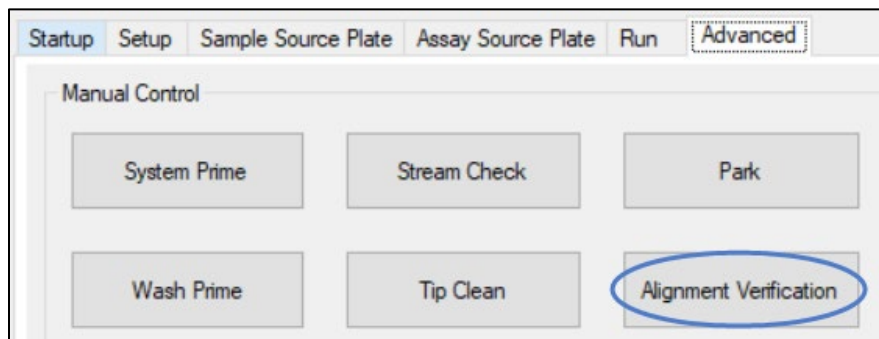


Figure 53. *Advanced* tab and [Alignment Verification] button.

NOTE: The other buttons on the *Advanced* tab located under the buttons shown in Figure 53 are reserved for use by a certified Field Service Engineer. Customers are discouraged from using these.

5. When dispensing is complete, evaluate the results. Inspect the alignment chip under UV light and magnification and note any fluorescent artifacts on the surface of the chip.

NOTE: Droplets on the upper edge of nanowell walls will sometimes appear to be outside of the nanowell. By changing the angle of illumination with the UV light, you should be able to better discriminate whether droplets are inside or outside of the nanowells.

- A few small artifacts on the surface of the chip are normal. Because the wells in the alignment chip are smaller than the wells on a standard SmartChip nanowell chip, the presence of a few small drops on the chip surface does not indicate that the system is out of alignment.
- If the number of fluorescent droplets outside the nanowells exceeds 16 (>1%), it may indicate that the system is out of alignment. Repeat the daily warmup procedure and alignment verification. If the problem persists, contact Takara Bio [technical support](#).
- Droplets may be present on the chip surface in a consistent direction (e.g., always on the right side of the wells), which may indicate misalignment. See Figure 54 (below) for an acceptable alignment verification run and one that warrants a call to Takara Bio [technical support](#).

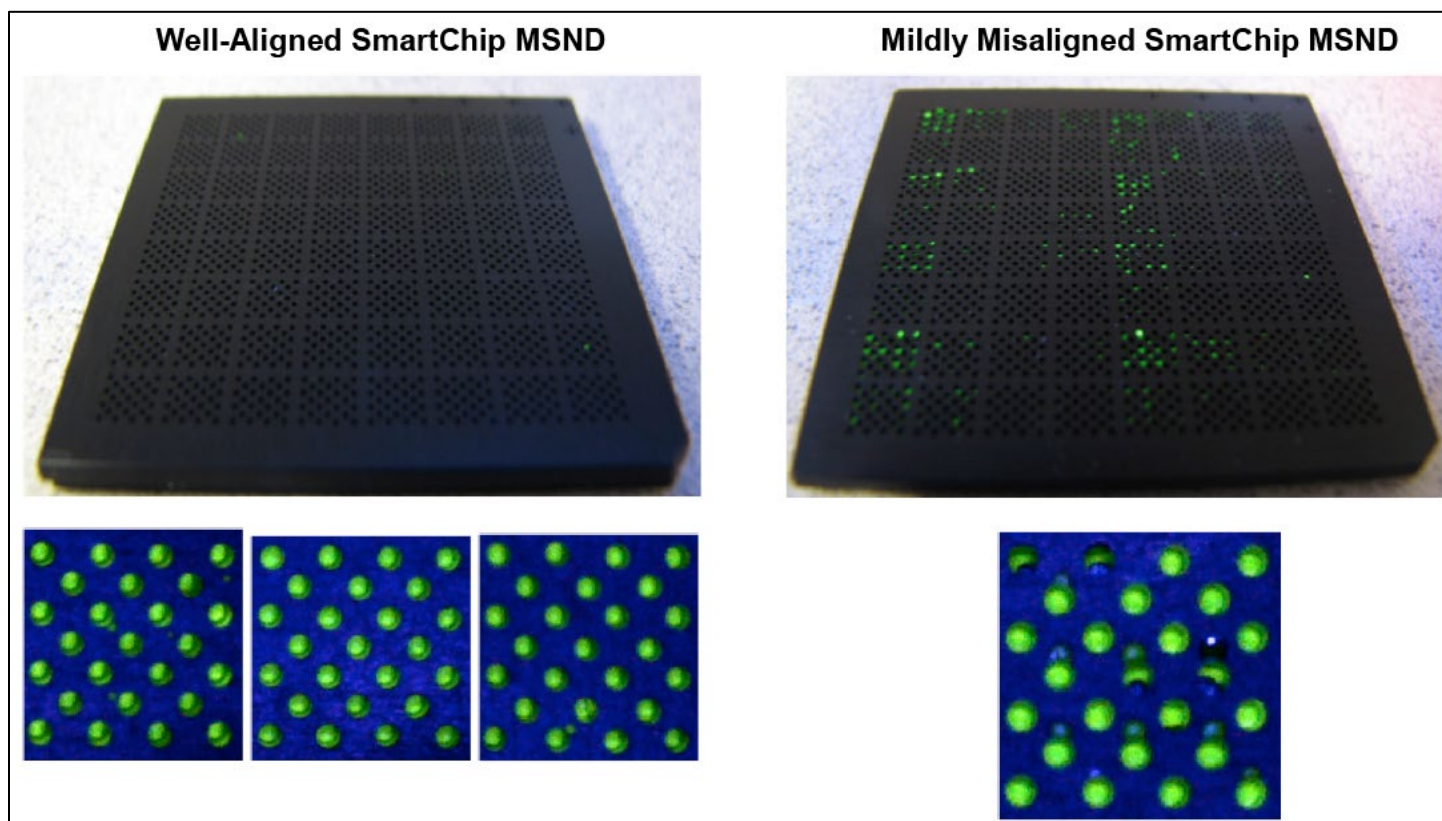


Figure 54. Alignment verification run results. In the photos on the left, some random droplets are visible. This is expected. In the photos on the right, droplets are consistently on the top side of the nanowells. This indicates misalignment.

6. Clean the alignment chip as follows:
 - a. Use the tab to carefully peel the film from the chip.
 - b. Thoroughly rinse the chip, first with deionized water, then with methyl, ethyl, or isopropyl alcohol.
 - c. Dry the chip with compressed air.

F. Remove Persistent Air Bubbles via Alcohol Wash Priming Procedure

Use this procedure to remove trapped bubbles from the syringes in the fluidic system as noted in Figure 20 (in Section V.F, "Run the Daily Warmup"). You will need ~500 ml of 70% isopropanol and a clean plastic bag to hold the fluidic harness during the procedure.

1. Put on clean gloves.
2. Open the top portion of the protective cover of the pressure reservoir, being careful not to damage the tubes coming from the lid.

3. Drain the water from the pressure reservoir and replace it with isopropanol, as described below.
 - a. Vent the noble gas by closing the stopcock on the noble gas input line and opening the vent stopcock (Figure 55).

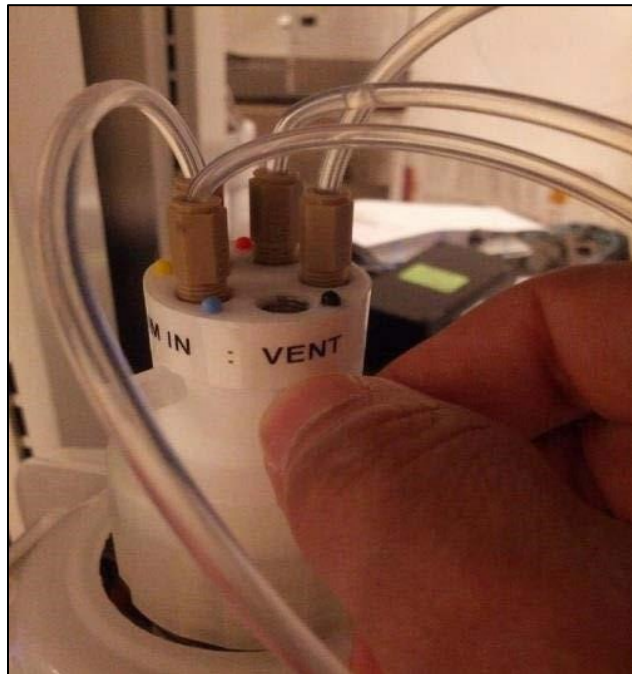


Figure 55. Venting the noble gas from the pressure reservoir.

- b. Carefully remove the cap and tubing from the pressure reservoir (Figure 56).



Figure 56. Removing the reservoir cap and tubing.

- c. Lift the fluidic harness, open the bag, and place the bag under the harness. Place the fluidic harness inside the bag and set it on the bench (Figure 57).



Figure 57. Fluidic harness.

- d. Empty the water from the pressure reservoir.
 - e. Fill the bottle with 500 ml of 70% isopropanol.
 - f. Reattach the cap and replace the tubes in the reservoir. Avoid touching the tubes when inserting them into the bottom of the reservoir.
 - g. Reattach the top of the protective cover.
 - h. Close the system by opening the stopcock on the noble gas input line and closing the vent stopcock.
 - i. Reattach the protective cover.
4. Prime the system with 70% isopropanol by running the first portion of the daily warmup procedure as described below.
 - a. Click the [Daily Warmup] button.
 - b. When the elapsed time is 55 sec, click the [Stop] button (Figure 58).



Figure 58. Elapsed time dialog box.

- c. When complete, repeat the prime procedure (Steps 4.a and 4.b) once more.
5. Run the daily warmup procedure (Section V.F).
6. Refill the reservoir with water as described below.
 - a. When the daily warmup is complete, depressurize the reservoir. Follow the instructions in Step 3 above to remove the fluidic harness. The same plastic bag can be used for this step.
 - b. After the fluidic harness has been removed, drain the remaining isopropanol from the reservoir to a waste container.
 - c. Rinse the reservoir thoroughly with deionized filtered (0.2 µm) water.
 - d. Fill the bottle with deionized filtered water to the top of the bottom section of the protective cover.
 - e. Let the reservoir liquid degas for 30 min. You should see noble gas bubbling through the water during this period.
 - f. Prime the system twice, following the instructions in Step 4 above.
7. Repeat the daily warmup procedure once more.

G. Common Replacement Parts

- External fuse (installed in the power entry module): 5 x 20 mm 5A Time Lag (Slo-Blo)
- Replace wash tubing in the peristaltic pump box with Flexelene tubing (Eldon James Company, Cat. No. FX1-2W)

H. Annual Preventative Maintenance

Have the SmartChip MSND examined and calibrated every year by a certified Takara Bio Field Service Engineer.

Appendix A. Troubleshooting

If the SmartChip MSND or SmartChip Dispenser Software does not respond as desired or a warning is displayed, please attempt to rectify the problem using the tables below. If you cannot solve the problem, please contact [technical support](#).

A. On Startup of Software, Dewpoint Controller Error is Displayed

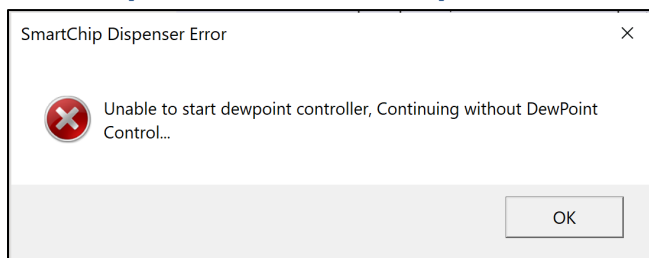


Figure 59. "Unable to start dewpoint controller" *SmartChip Dispenser Error* pop-up message.

Table 15. Problem: On startup of software, dewpoint controller error is displayed (Figure 59)

Possible cause	Solution
----------------	----------

Connection to pump control box not properly re-established	Close the software. Unplug the pump control box USB cable from the laptop and plug it back in. After the connection has been re-established, restart the software.
--	--

Table 16. Problem: Hanging drop, drop dispersion, or improper dispensing.

Possible cause	Solution
Trapped air in the system fluidics	A large volume of air in the tube will act like a spring. When the microsolenoid valve is actuated, the air will absorb the pulse, leaving a drop hanging on the end of the tip. Inspect the tube between the tip and the 2 x 6 manifold (where not covered). Look for air or bubbles within the tube. If air is found within the tube, move the tips to the wash position and prime the system by clicking the [Daily Warmup] button.
Faulty tip connection	Inspect the slip fits on the tips and on the 2 x 6 manifold. The tubing must fit snugly to the stainless-steel tube. If the tube can be removed easily, cut off a small section of the tube and reseal the tube.
Crimped fluidic tubing	Inspect the tubing for crimps or bends. Remove crimped/bent sections if feasible or replace the harness.
Plugged tip	Backflush the tips by clicking the [Tip Clean] button in the SmartChip Dispenser Software. If the tip is plugged with a soluble material, aspirating and dispensing reagent capable of dissolving the material may clear the blockage. If these measures fail, it may be necessary to replace the tip, or the blockage could be upstream of the tip. Contact Takara Bio technical support.
Leaking inlet valve	Let the system sit idle for 5 min and inspect the dispensing tips. If there are water bubbles at any of the tips, the corresponding solenoid is leaking. Contact Takara Bio technical support.
Incompatible buffers and samples	Extremes of fluidic properties, such as viscosity, may result in poor performance. Contact Takara Bio technical support.
Tubing in the pump box is cracked	Replace existing Wash tubing with Flexelene tubing (Eldon James Company, Cat. No. FX1-2W).

B. Low Pressure Error Displayed

Table 17. Problem: Low Pressure error displayed.

Possible cause	Solution
Pressure is too low	Check that the noble gas supply regulator is set to 30 psig (2 Bar) maximum for a standard system. If problem persists, contact Takara Bio technical support.

C. Dispensing Head Does Not Home

Table 18. Problem: Dispensing head does not home.

Possible cause	Solution
No communication with the instrument	Cycle the power on the fluidic module and restart the computer.

D. Low or Partial Dispenses

Table 19. Problem: Low or partial dispenses.

Possible cause	Solution
Microsolenoid valve failure	Contact Takara Bio technical support.

Relative height of system components	The relative height of the pressure reservoir, stage module, and fluidic module must be the same as when the system was installed. If you change the height of any component and are seeing low or partial dispenses, contact Takara Bio technical support.
Crimped tubing	See "Hanging drop" (Table 16) above.
Pressure too low	See Table 17, above.

E. Apparent Low Sample Concentration

Table 20. Problem: Apparent low sample concentration.

Possible cause	Solution
Syringe thumbscrew is loose	Tighten the syringe thumbscrew until finger tight. The thumbscrew is located at the bottom of the syringe in the fluidic module.
Tip is plugged	See "Hanging drop" (Table 16) above.
Air bubble in the syringe path	Prime the syringe path by performing the daily warmup.
Microsolenoid valve is leaky	See "Hanging Drop > Leaking inlet valve" (Table 16) above.
Syringe valve is blocked or leaky	See "Hanging Drop > Leaking inlet valve" (Table 16) above.
Low liquid level in the pressure reservoir	Check the level of the system liquid in the pressure reservoir. Make sure that the end of the tubing is submerged in the water. Add deionized, degassed water as needed (see "Refill the Pressure Reservoir," Section V.D).

F. System Stalls Because the Syringe Does Not Move

Table 21. Problem: System stalls because the syringe does not move.

Possible cause	Solution
No power	Inspect the power cables and connections.
Syringe is not initialized	Cycle the power on the fluidic module and restart the computer.
Obstruction	Verify that the syringes are not obstructed.

G. Persistent Soft Clicking

Table 22. Problem: Persistent soft clicking. The digital pressure regulator in the fluidic module has a soft click during normal operation to maintain pressure.

Possible cause	Solution
Noble gas leak in the system	<p>Place soapy water around the following gas connections in the system:</p> <ul style="list-style-type: none"> • 5-port cap connection to the pressure reservoir • All 5-port cap ports • Inlet and outlet of pressure relief valve • Gas outlet connection at the back of the fluidic module • Gas inlet connection at the back of the fluidic module • Noble gas tank connections <p>Bubbles are an indication of a leak at that connection. Tighten the fitting.</p> <p>Check for holes in the tubing from the gas outlet of the fluidic module into the noble gas input ports (normally the green and blue ports of the pressure reservoir).</p> <p>Check that the O-ring underneath the 5-port cap is seated correctly.</p>

Ensure that the stopcock for the vent port on the pressure reservoir is in the closed position (i.e., the back port is closed on a standard pressure bottle).

Ensure that the ferrule orientations for the noble gas input ports on the pressure reservoir are correct.

H. Loud Digital Pressure Regulator Chattering

Table 23. Problem: Loud digital pressure regulator chattering.

Possible cause	Solution
Gas path blocked at the pressure reservoir inlet	Ensure that the stopcock for the standard noble gas input port on the pressure reservoir is in the open position (this is the blue port on a standard reservoir bottle and should be in the vertical position). Verify that the input pressure from the noble gas tank regulator is in the appropriate range and not too high.

I. Soft Clicking from the Digital Pressure Regulator, Fluid Leak Observed

Table 24. Problem: Soft digital pressure regulator clicking and fluid leak observed.

Possible cause	Solution
Fluid leak in the system downstream of the noble gas input	<p>Locate the source of the leak. Tighten the fittings and tubing at the source of the leak. Possible sources include the following:</p> <ul style="list-style-type: none"> Liquid output ports on the pressure reservoir (red and yellow ports on a standard bottle). Check that the fittings are tight and that the ferrule orientations are correct. 8-port manifold Hole in tubing Connections at the microsolenoid valve Anywhere in the syringe or pressure paths

Appendix B: Preparing Source Plates

A. Preparing Source Plate Files in a Text Editor

Source plate files describe the contents of the 384-well source plates that the SmartChip MSND draws from to fill SmartChip Panels or MyDesign chips. These files describe sample or PCR assay attributes and their locations in the plate. This appendix describes how to create these files in a text editor.

To create your own source plate files

Source plate files must be text (*.txt) files. The first part of the file contains header information that should not be modified; the rest of the file is composed of tab-delimited rows of text describing the well contents, with one row for each well. We recommend that you copy the format from the appropriate source plate template file that is installed with the SmartChip Dispenser Software, and then modify the copy (see Step 1, below)

Keep the following in mind when creating a source plate file:

- Valid sample and assay names can contain alphanumeric characters (a-z, 0-9,) hyphens (the - symbol), and underscores (the _ symbol). Do not use forward slashes (/).
- Spaces ([Space bar]) should not be used within the data fields, as it may cause issues that invalidate the file information.

- Always use [Tab] as a column separator, i.e., a tab-delimited file.
- For the 6 assay X 768 samples dispense pattern, only one file is used. All 768 samples should be included in that file.

NOTE: We strongly recommend that you do not use Notepad to create or edit source plate files. Tab-delimited formatting is difficult to see in Notepad, making it easy to introduce formatting errors while editing. Microsoft Excel or text editors such as Notepad++ display tab-delimited text better.

1. In MS-Excel or a text editor of your choice (see **NOTE**), open the source plate template file corresponding to the type of source plate you want to document.

The template files are found in the following directory:

```
C:\ProgramData\takara\SmartChipDispenser
```

and there are separate `Templates` folders for assay and sample source plate files:

```
SmartChipDispenser\Assay Source plate files\Templates
```

```
SmartChipDispenser\Sample Source plate files\Templates
```

The filename conventions for the source plate template files are:

- MD (for MyDesign) or PD (predispensed)
- Number of PCR assays in the SmartChip layout (e.g., 12) followed by an 'A' for assay (e.g., 12A, 48A, 72A)
- Number of replicate PCR assays (e.g., 1 for SNP genotyping, 4 for gene expression analysis) followed by an 'R' for replicate (e.g., 1R, 4R)
- Number of samples (e.g., 3) followed by an 'S' for sample (e.g., 3S, 12S)
- Source plate type (e.g., `Sample_Sourceplate_File` or `Assay_Sourceplate_File`)
- File extension (*.txt)

Each grouping (except the file extension) is connected to the others by an underscore (_).

Example:

The file:

```
MD_12A_1R_384S_Sample_Sourceplate_File.txt
```

is for a MyDesign chip with 12 PCR assays, 1 replicate (indicating genotyping), and 384 samples for a sample source plate.

2. Add your source plate information below the text "Begin sample (assay) information" and after the header (column labels).

The source plate description information at the top of the file, the header (column label) text, and the numbers in the "Source" or "Well" column are required by the software. Type your information below the header using tabs to separate columns of information (see "Attributes for Sample Source Plate Files" and "Attributes for Assay Source Plate Files", Tables 24–27, below)

NOTES:

- **Do not edit the "Header" text in the template file.** The software will not find your information if you change the headings (column labels) in your source plate files.

- **Do not change the information in the "Source" column.** This column gives the locations of your sample mixtures or assays in the 384-well source plate and cannot be changed. The SmartChip MSND requires that samples and assays be in certain wells of the source plate in order to properly fill the different layout options for SmartChip Panels or MyDesign chips.

3. Save your source plate file in the folders:

SmartChipDispenser**Assay Source plate files**\

or:

SmartChipDispenser**Sample Source plate files**\

depending on the type of source plate used. Do NOT save the file in the original Templates folder.

Give the file a descriptive name.

The sample and assay attributes that can be entered for the two types of analysis (gene expression and SNP genotyping) are shown below.

Gene expression analysis source plates

Table 25. Attributes for sample source plate files for gene expression analysis.

SampleName	Concentration	Source
(Required)	(Optional)	(Do not change!)

The list below explains the purpose of each column/header:

- **SampleName: (Required)** The name of the sample.
- **Concentration: (Optional)** This is the concentration information of the sample
- **Source:** This is a numerical code assigned to each well of the 384-well source plate. These must be in order, so should NOT be modified.

Example:

SampleName	Concentration	Source
Sample_A1	500pg	1
Sample_A2		2
Sample_B1	1ng	3

Table 26. Attributes for assay source plate files for gene expression analysis.

AssayName	Source	AssayID	Tm	IsHousekeeping
(Required)	(Do not change!)	(Required)	(Optional)	(Optional)

The list below explains the purpose of each column/header:

- **AssayName: (Required)** The name of the assay.
- **Source:** This is a numerical code assigned within the software to each well of the 384-well source plate. These should NOT be modified.
- **AssayID: (Optional)** This is the ID value assigned to the assay.
- **Tm: (Optional)** the expected amplicon melting temperature for the sample, which can be used at the end of the assay to measure specificity
- **IsHousekeeping: (Optional)** This field indicates whether or not the assay is a reference gene product assay. Accepted values are either 'yes' or 'no' (without quotes).

Example:

AssayName	Source	AssayID	Tm	IsHousekeeping
GAPDH	1	24	72	yes
Assay_Y2	2	27	68	no
Assay_Z3	3	42		no

SNP genotyping source plates

Table 27. Attributes for sample source plate files for SNP genotyping.

SampleName	Concentration	Source	Gender	Population	Custom 1	Custom 2
(Required)	(Optional)	(Do not change!)	(Optional)	(Optional)	(Optional)	(Optional)

The list below explains the purpose of each column/header:

- **SampleName: (Required)** The name of the sample.
- **Concentration: (Optional)** This is the sample DNA concentration information.
- **Source:** This is a numerical code assigned within the software to each well of the 384-well source plate. These should NOT be modified.
- **Gender: (Optional)** This field can be used to associate the gender information of the sample DNA with the sample in the results files.
- **Population: (Optional)** This field can be used to associate population information of the sample DNA with the sample in the results files.
- **Custom1, Custom2: (Optional)** These fields can be used to record additional information you want to associate with the samples through to the results files.

Table 28. Attributes for assay source plate files for SNP genotyping.

ID	Source	Name	Species	Gene Symbol	Category ID
(Required)	(Do not change!)	(Required)	(Optional)	(Optional)	(Optional)

The list below explains the purpose of each column/header:

- **ID: (Required)** The ID value assigned to the assay.
- **Source:** This is a numerical code assigned within the software to each well of the 384-well source plate. These should NOT be modified.
- **Name: (Required)** The name of the assay.
- **Species: (Optional)** The species the sample/gene is taken from.
- **Gene symbol: (Optional)** The symbol assigned to the target gene.
- **Category ID: (Optional)**

B. Workflow Guidelines for 768-Sample Dispense (MyDesign)

! **IMPORTANT:** This pattern requires the user to load two 384-well source plates with samples (768 wells total) back-to-back. **Prepare both plates before initiating dispense.**

1. Generate a sample source plate layout file and load into the *Sample Source Plate* tab for Plate 1 and Plate 2 (see Section VII.C for more information).

NOTE: We advise users to print the sample source plate maps from this tab to facilitate loading of plates.

2. Label the 384-well plates to identify "Plate 1" and "Plate 2" (as designated in the *Sample Source Plate* tab).
3. Load the 384-well plates with samples by referring to the sample source plate map (Step 1 note).
4. After each 384-well plate is filled, seal with adhesive film from MSND 384-Well Source Plate and Seals and centrifuge at 3,220g for 5 min at room temperature.
5. Remove seal from Plate 1, load the plate into the SmartChip MSND, and initiate "Plate 1 Samples" dispense (Figure 60).

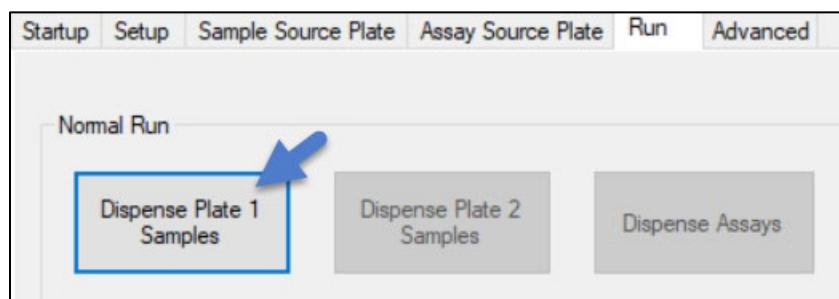


Figure 60. The [Dispense Plate 1 Samples] button on the *Run* tab for the 6 assays X 768 samples layout.

6. Immediately after this dispense completes, remove Plate 1 from the multiwell plate nest and discard appropriately. Remove the seal from Plate 2 and load it into the plate nest.
7. Click the [Dispense Plate 2 Samples] button.
8. After the Plate 2 sample dispense completes, proceed to the assay dispense (Section VIII.D) and continue with the protocol in Section VIII.

C. Guidelines for Partially Filled 384-Well Source Plates or Plates Filled by Automation

The SmartChip MSND collects source material for dispense in a 2 x 4 pattern across the 384-well plate—two columns and four rows, when in landscape orientation—and it's recommended that it not be programmed to aspirate from empty source wells to protect the functionality of the instrument.

If the number of assays and/or samples dictates a 384-well plate source map with empty source wells, we suggest adding 1X TE solution into all wells the MSND dispense tips might interact with. These cases might include:

- When dispensing samples or assays from a 96-well plate into the 384-well plate using an automated pipette.

- If you have a number of samples that does not exactly match any of the preset dispense patterns. For example, if you have 100 samples and are using a MyDesign chip, you should choose the 108 samples option and fill the final 8 "sample" wells with 1X TE solution.

Figures 61–63 will help determine which wells should be filled when using automation. This is also covered in the onsite training by the Field Application Scientist upon receipt of the SmartChip system.

NOTE: If you have any questions about customizing the number of samples or assays or how they're distributed in the source plate beyond what is covered in this section and the next (Section C), please contact [technical support](#).

Example source well plate map for automated pipette use

In Figure 61, there are 67 samples (indicated by the purple boxes) planned to be dispensed by an automated pipette into the 384-well source plate in alternating columns and rows, out to Column 17, Rows A, C, and E.

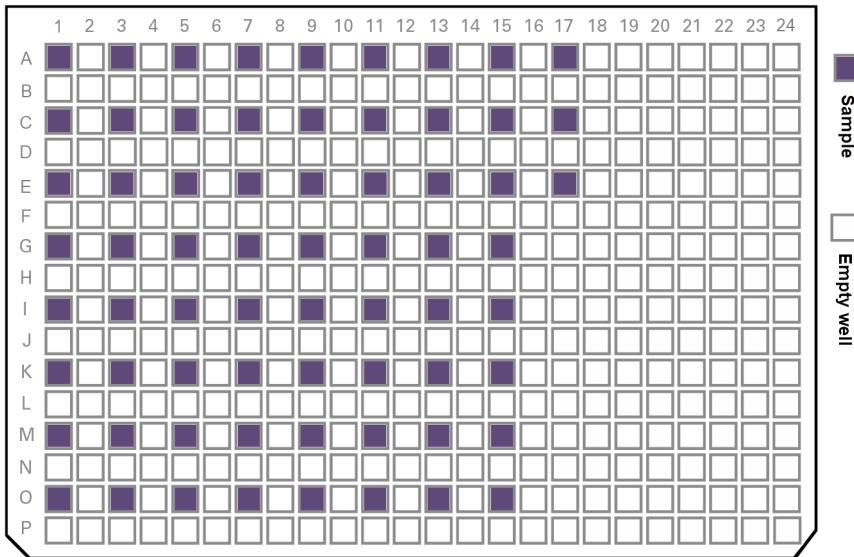


Figure 61. A 384-well plate containing 67 samples as will be dispensed using automation.

1X TE solution should be added to empty wells that the SmartChip MSND will aspirate to in a 2 x 4 grid; that grid is overlaid on the plate in Figure 62.

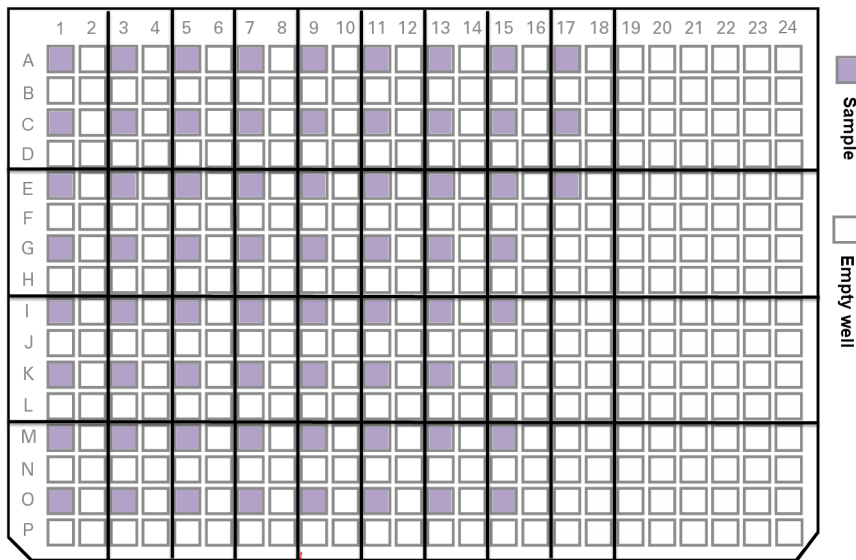


Figure 62. A 384-well plate containing 67 samples with the MSND aspiration grid overlaid.

Each grid area consists of eight wells. In the example in Figure 62, there are 34 grid areas that contain samples, which translates to 272 wells (34 x 8) in those grid areas.

Since 272 wells doesn't match one of the preset combinations for sample dispense, the dispense coverage would need to be rounded up to the max 384 wells (the '384 samples x 12 assay' dispense preset would therefore need to be selected when preparing to dispense).

The final plate map would therefore resemble Figure 63.

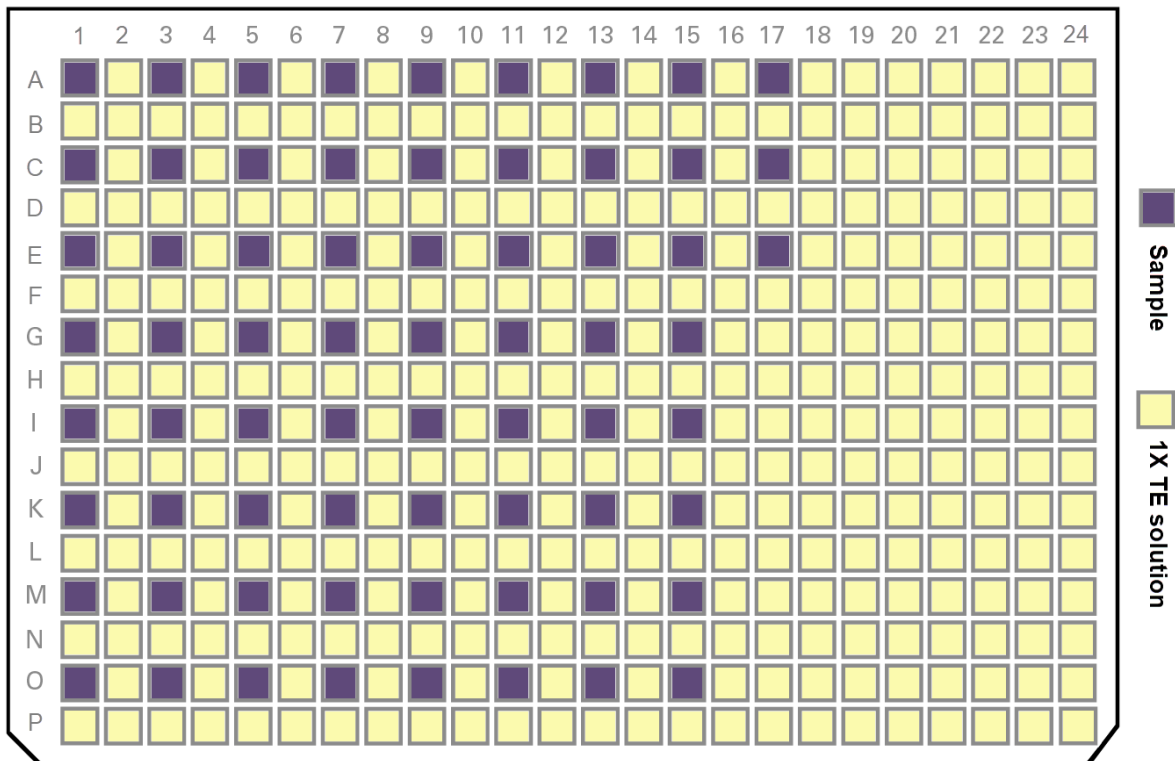



Figure 63. The 384-well source plate fill map for 67 samples dispensed by an automated pipette + 1X TE solution to accommodate the SmartChip MSND best practice.

D. Printable 384-Well Source Plate Maps

Notes about using the plate maps below:

- The image to the right (yellow background with 'TE' text) is used in the plate maps to indicate wells that require being filled with a 1X TE solution (or equivalent) for a given sample preset in order to accommodate the SmartChip MSND best practices (described in the previous section). 
- If you have a number of samples that does not exactly match any of the preset dispense patterns, round up to the next sample number preset that will include all your samples, and then fill the unused "sample" wells with 1X TE solution. These "sample" wells filled with 1X TE solution would be in addition to any wells requiring 1X TE solution, as determined by the best practice.

NOTE: If you have questions about doing this that are not answered by this point or in the previous section (Section B), please contact [technical support](#).

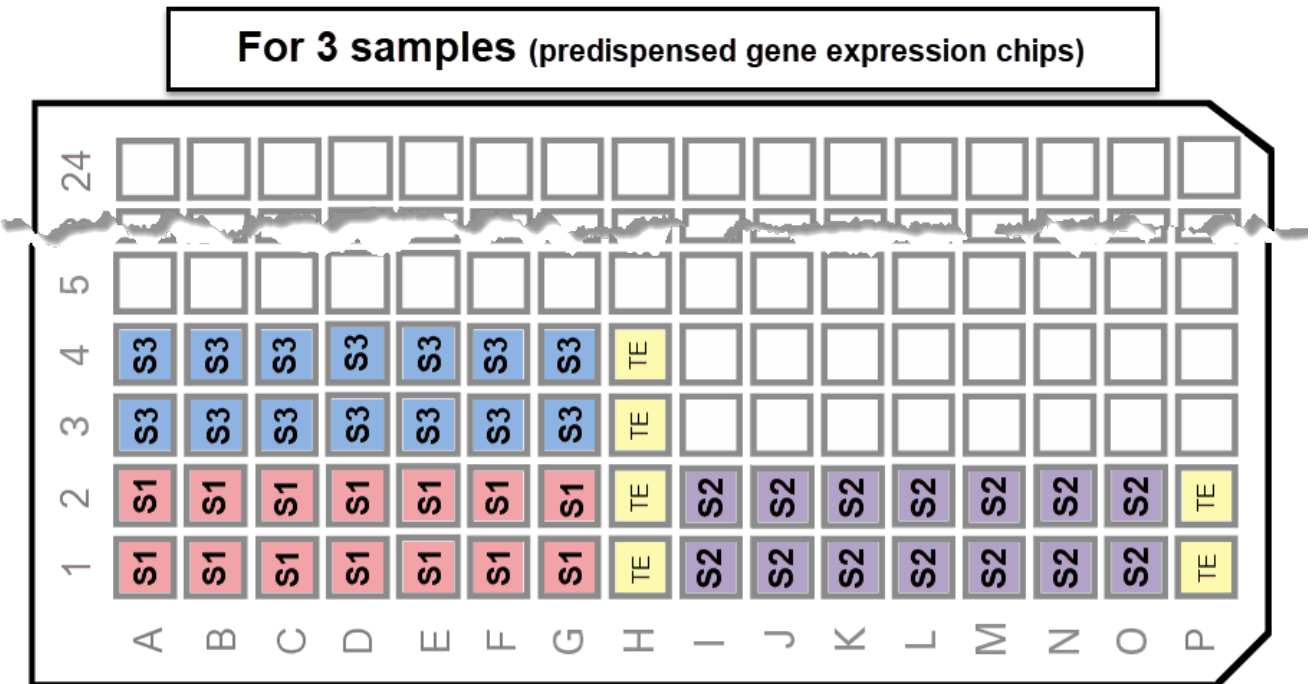


Figure 64. Printable 384-well plate map (partial) for dispense of 3 samples into a predispensed chip for gene expression panels.

For 6 samples (predispensed gene expression chips)

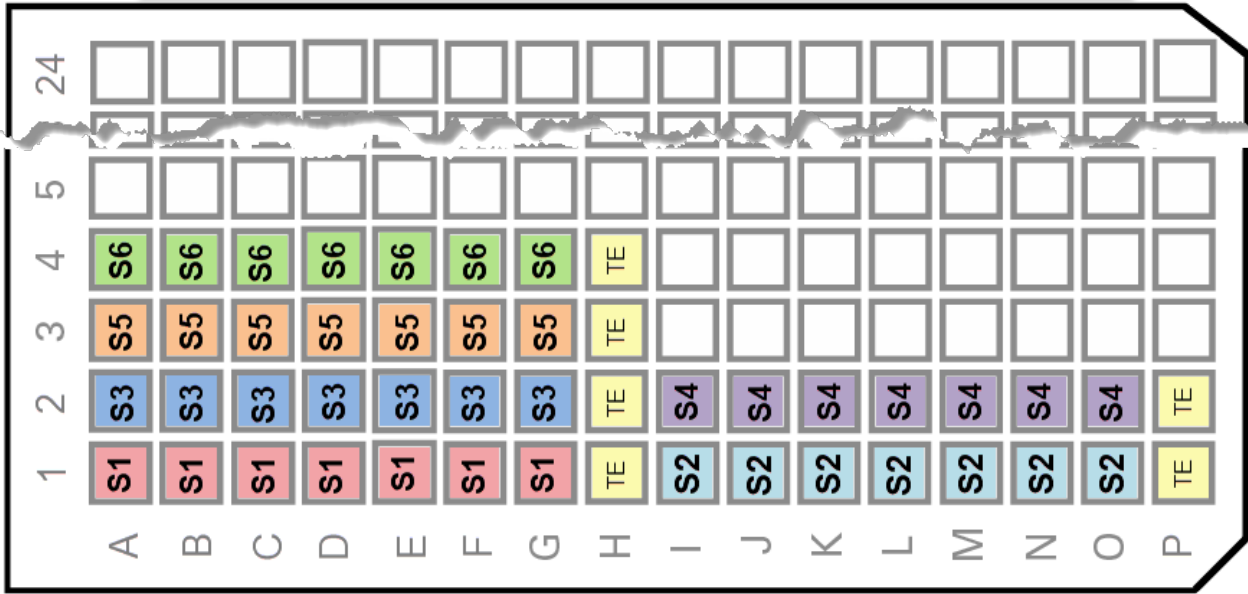


Figure 65. Printable 384-well plate map (partial) for dispense of 6 samples into a predispensed chip for gene expression panels.

For 12 or 16 samples or assays

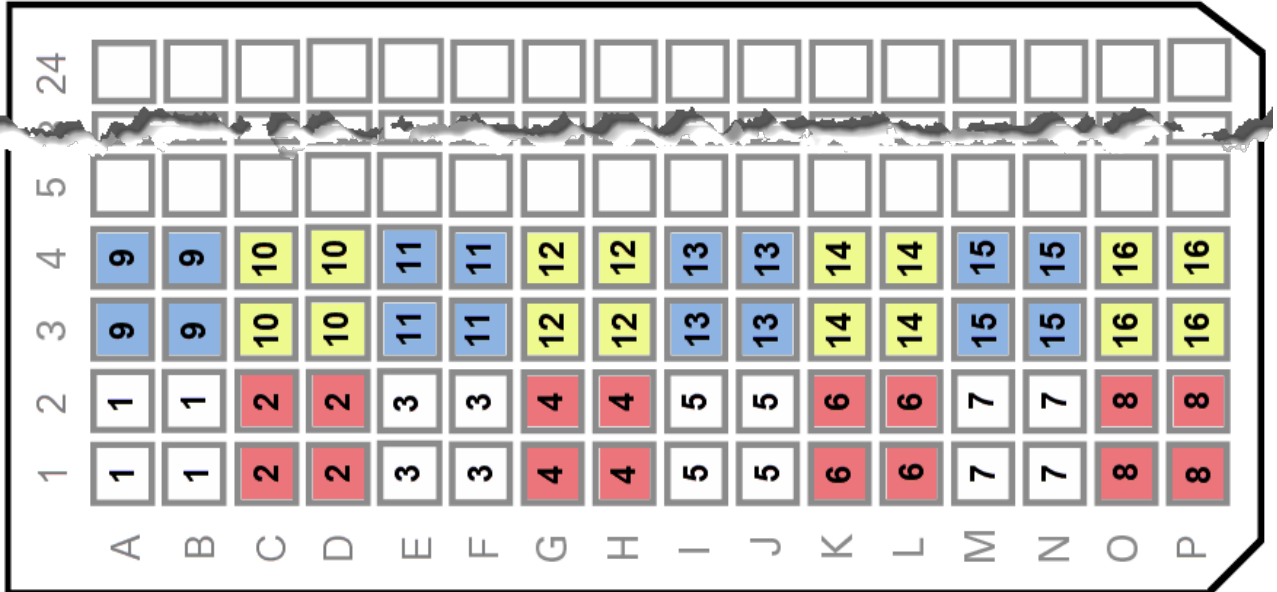


Figure 66. Printable 384-well plate map (partial) for dispense of 12 or 16 samples or 12 assays.

20 samples

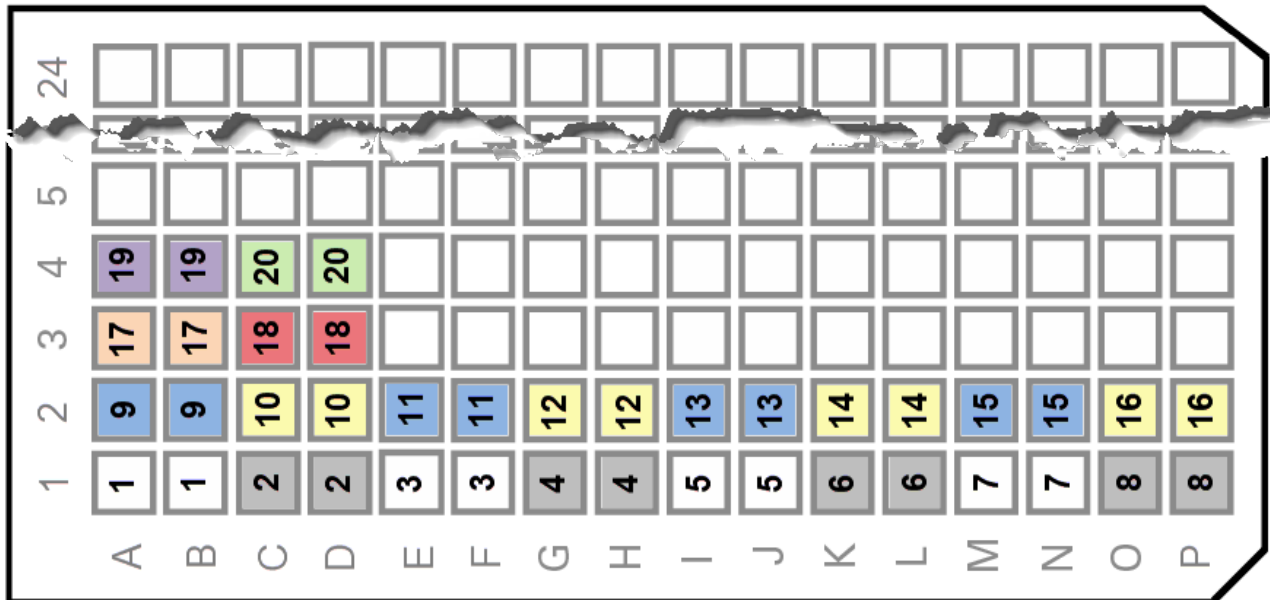


Figure 67. Printable 384-well plate map (partial) for dispense of 20 samples.

24 samples or assays

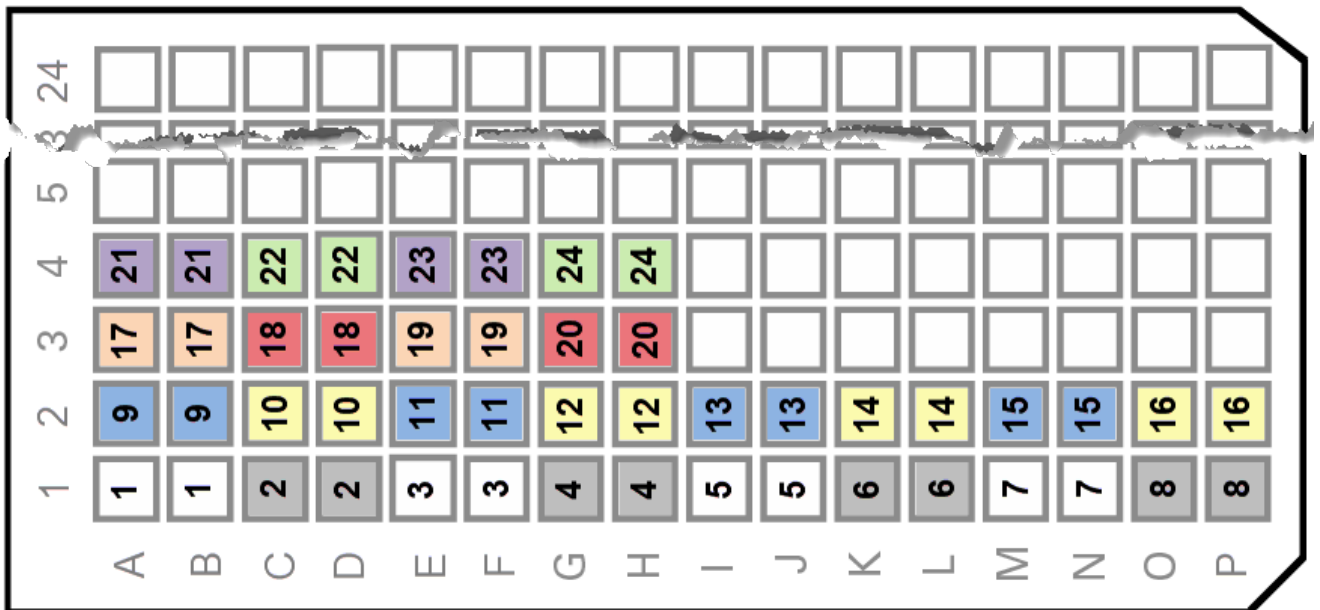


Figure 68. Printable 384-well plate map (partial) for dispense of 24 samples or assays.

For 36 samples or assays

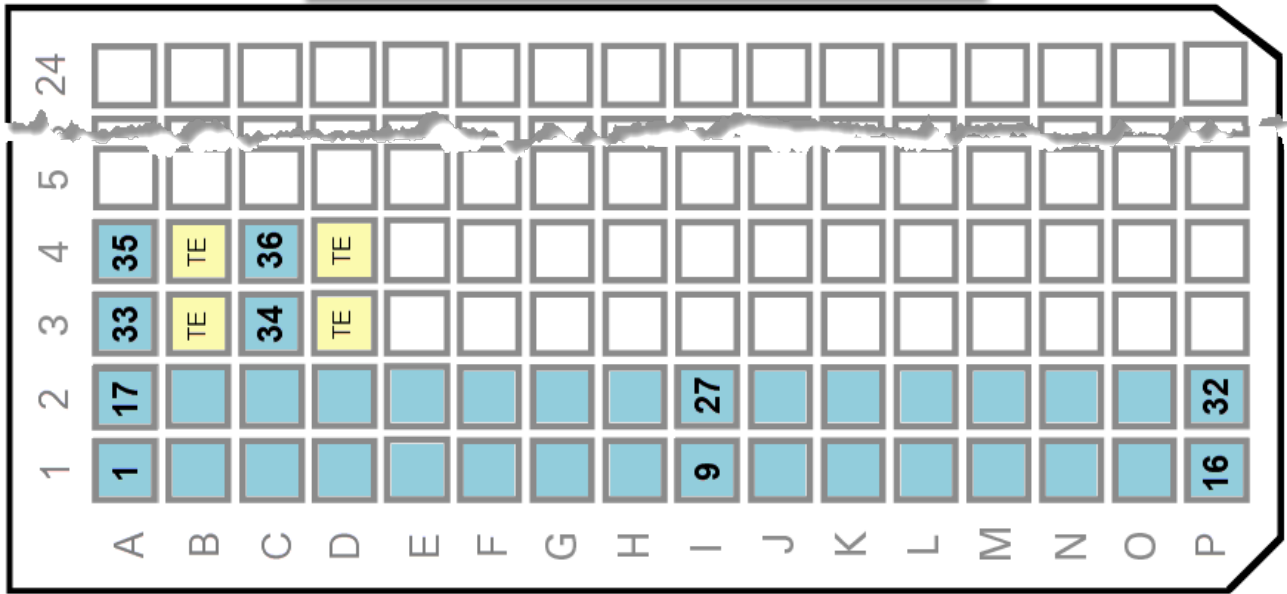


Figure 69. Printable, partial 384-well plate map for dispense of 36 samples or assays.

For 42 samples

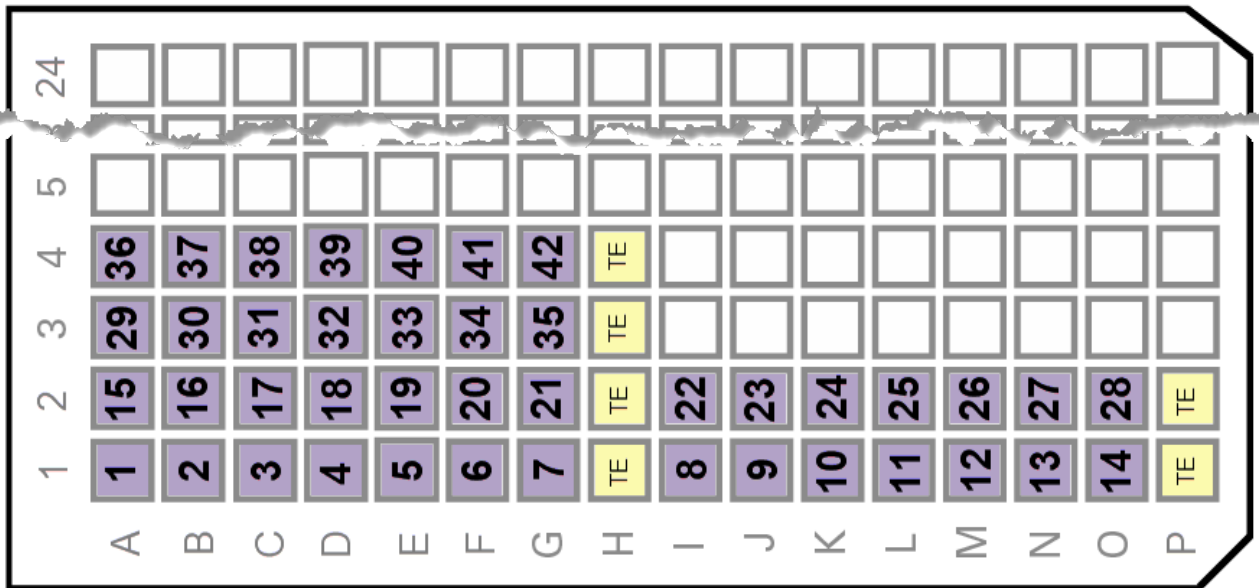


Figure 70. Printable 384-well plate map (partial) for dispense of 42 samples into a predisposed chip for SNP genotyping panels.

For 48 samples or assays

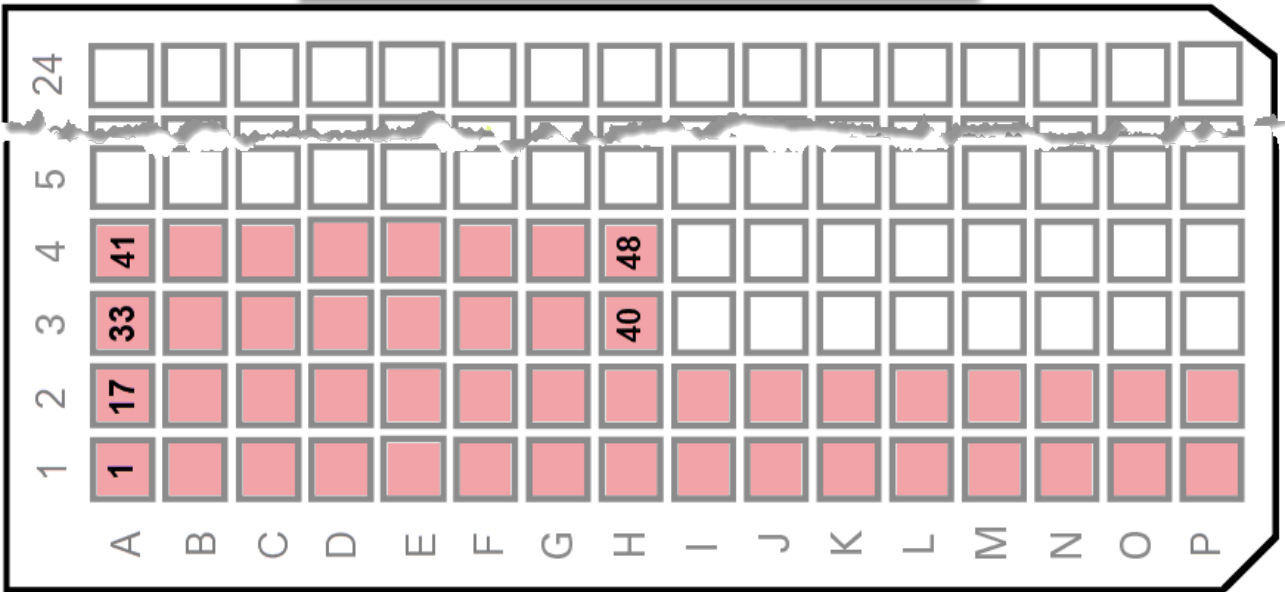


Figure 71. Printable, partial 384-well plate map for dispense of 48 samples or assays.

For 54 samples or assays

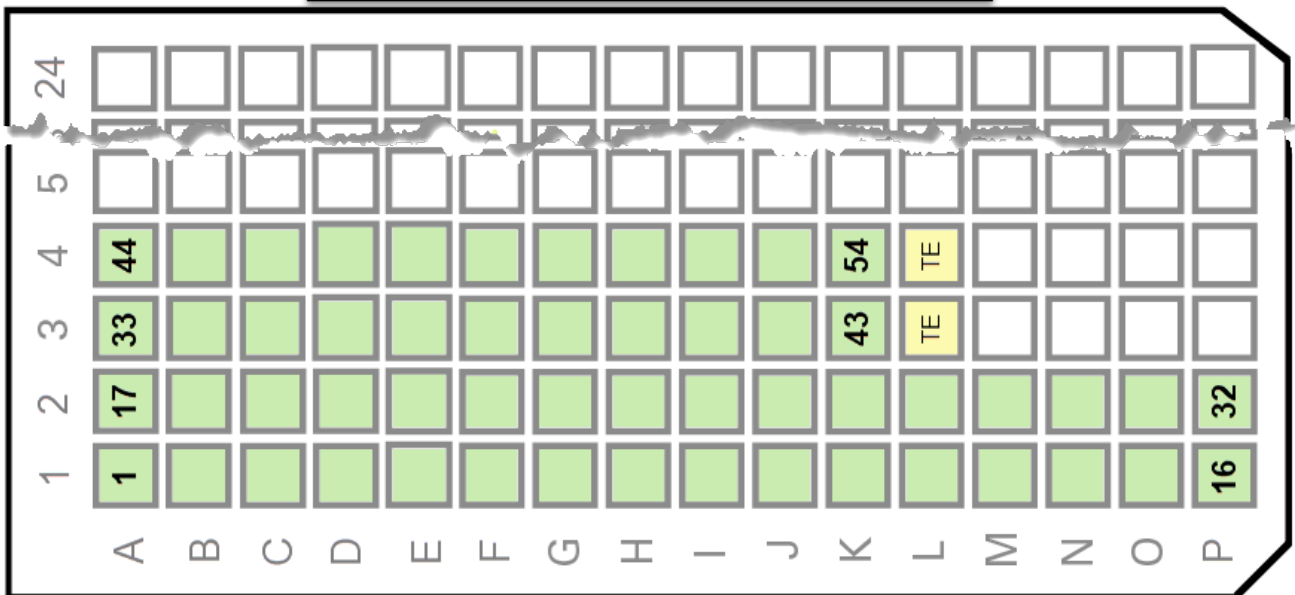


Figure 72. Printable, partial 384-well plate map for dispense of 54 samples or assays.

64 or 96 samples or assays

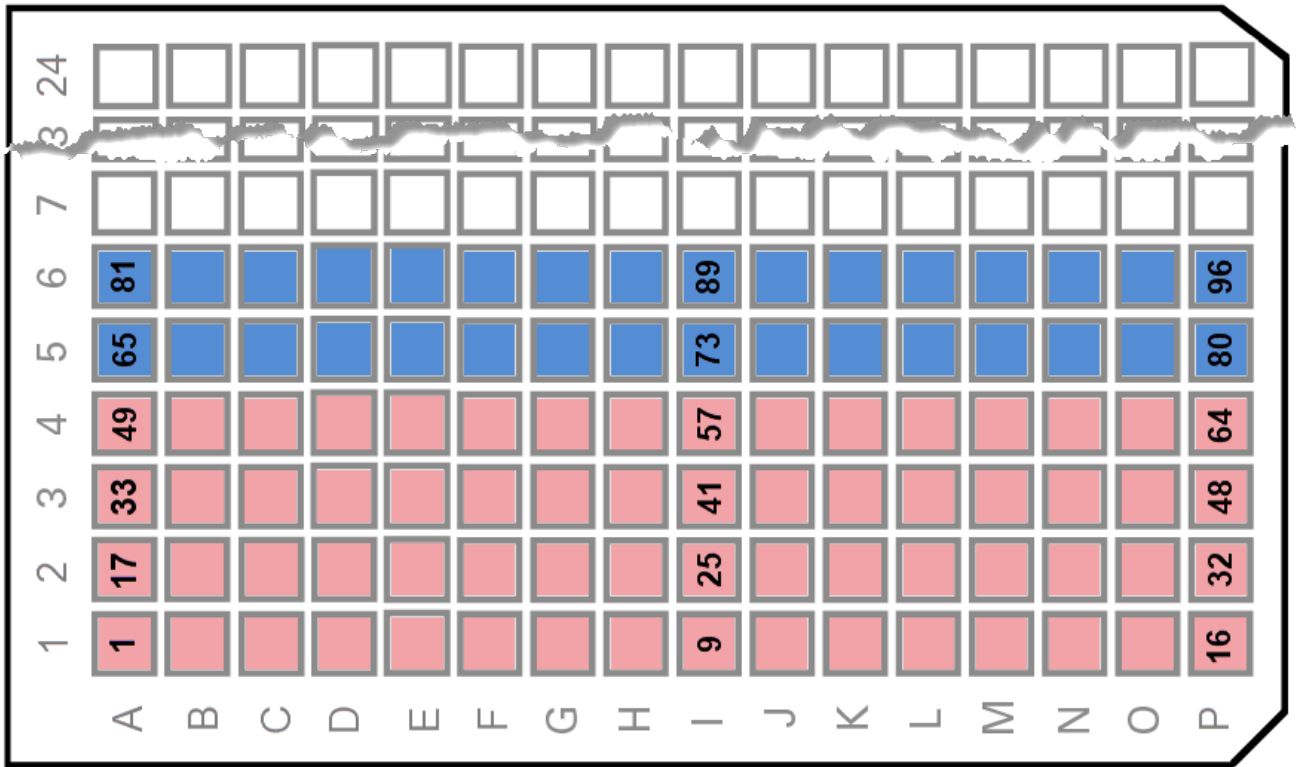


Figure 73. Printable, partial 384-well plate map for dispense of 64 or 96 samples or assays.

72 samples or assays

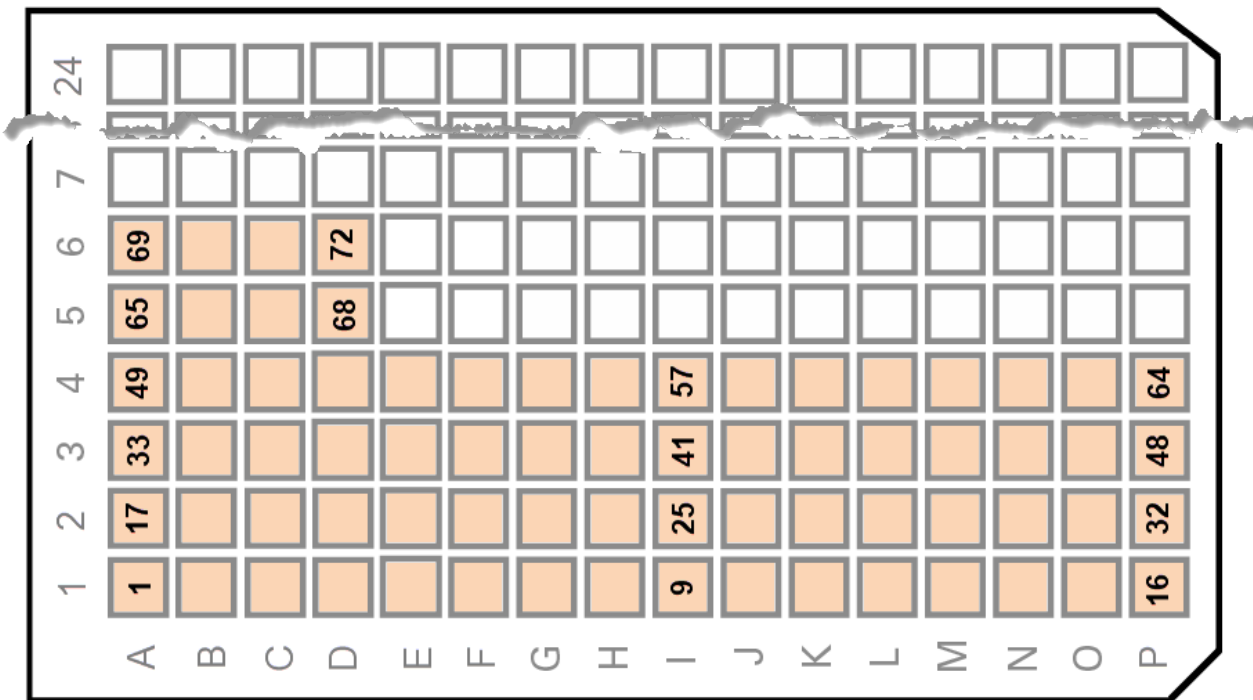


Figure 74. Printable, partial 384-well plate map for dispense of 72 samples or assays.

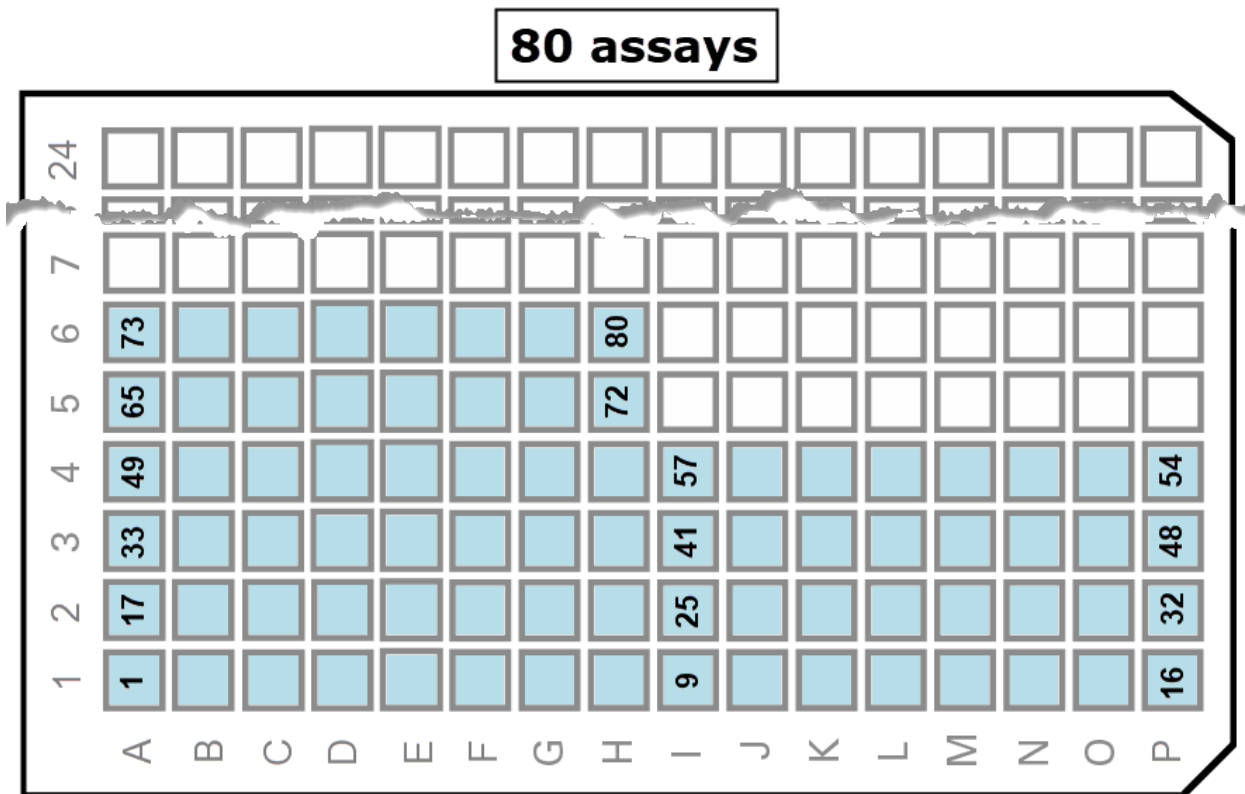


Figure 75. Printable, partial 384-well plate map (partial view) for dispense of 80 assays.

For 108 samples

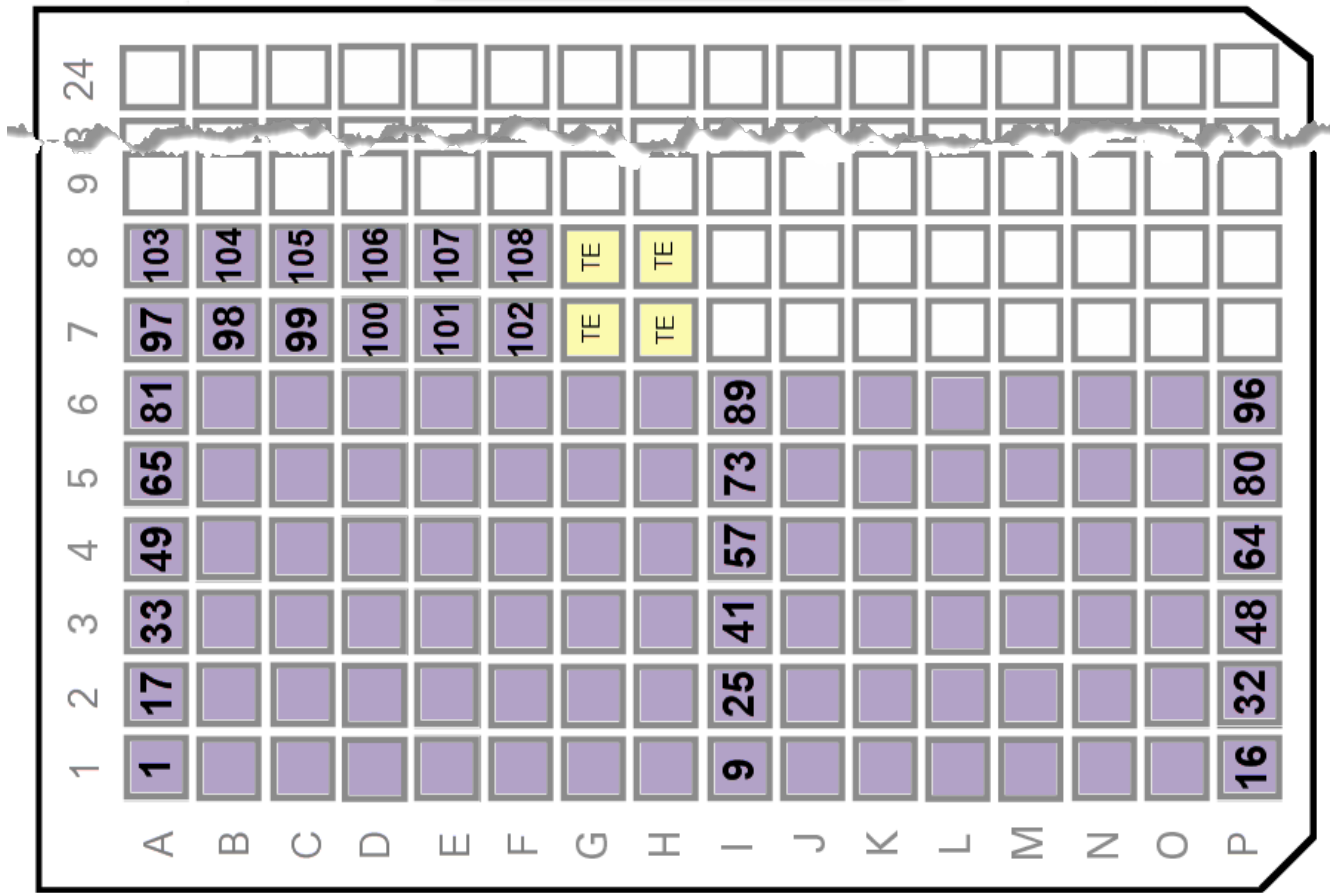


Figure 76. Printable 384-well plate map (partial view) for dispense of 108 samples.

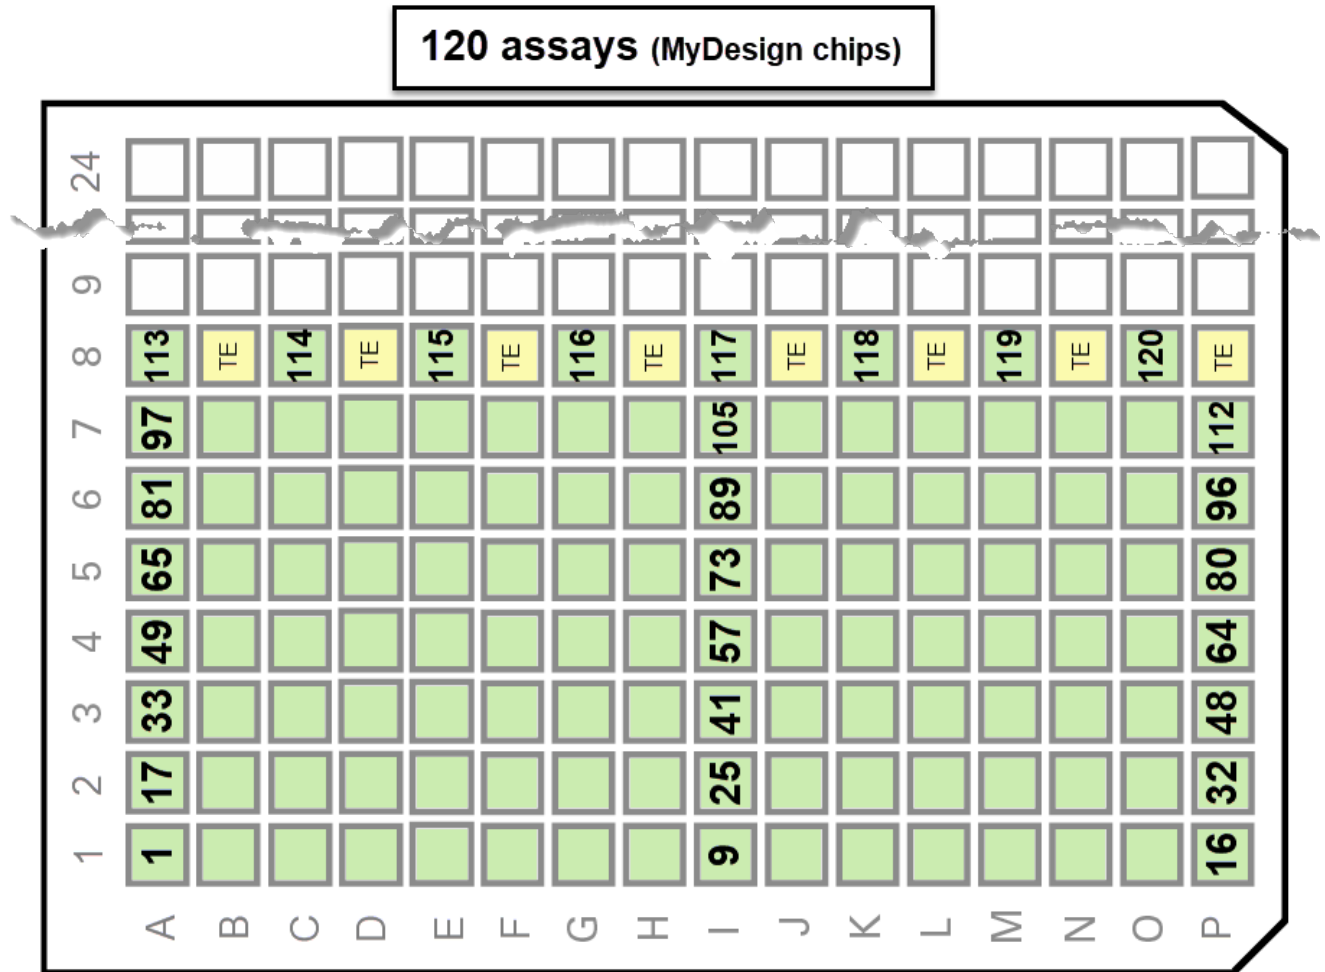


Figure 77. Printable 384-well plate map (partial) for dispense of 120 assays into a MyDesign chip.

144 samples or assays



Figure 78. Printable 384-well plate map (partial) for dispense of 144 samples or assays into a MyDesign chip.

For 216 samples or assays

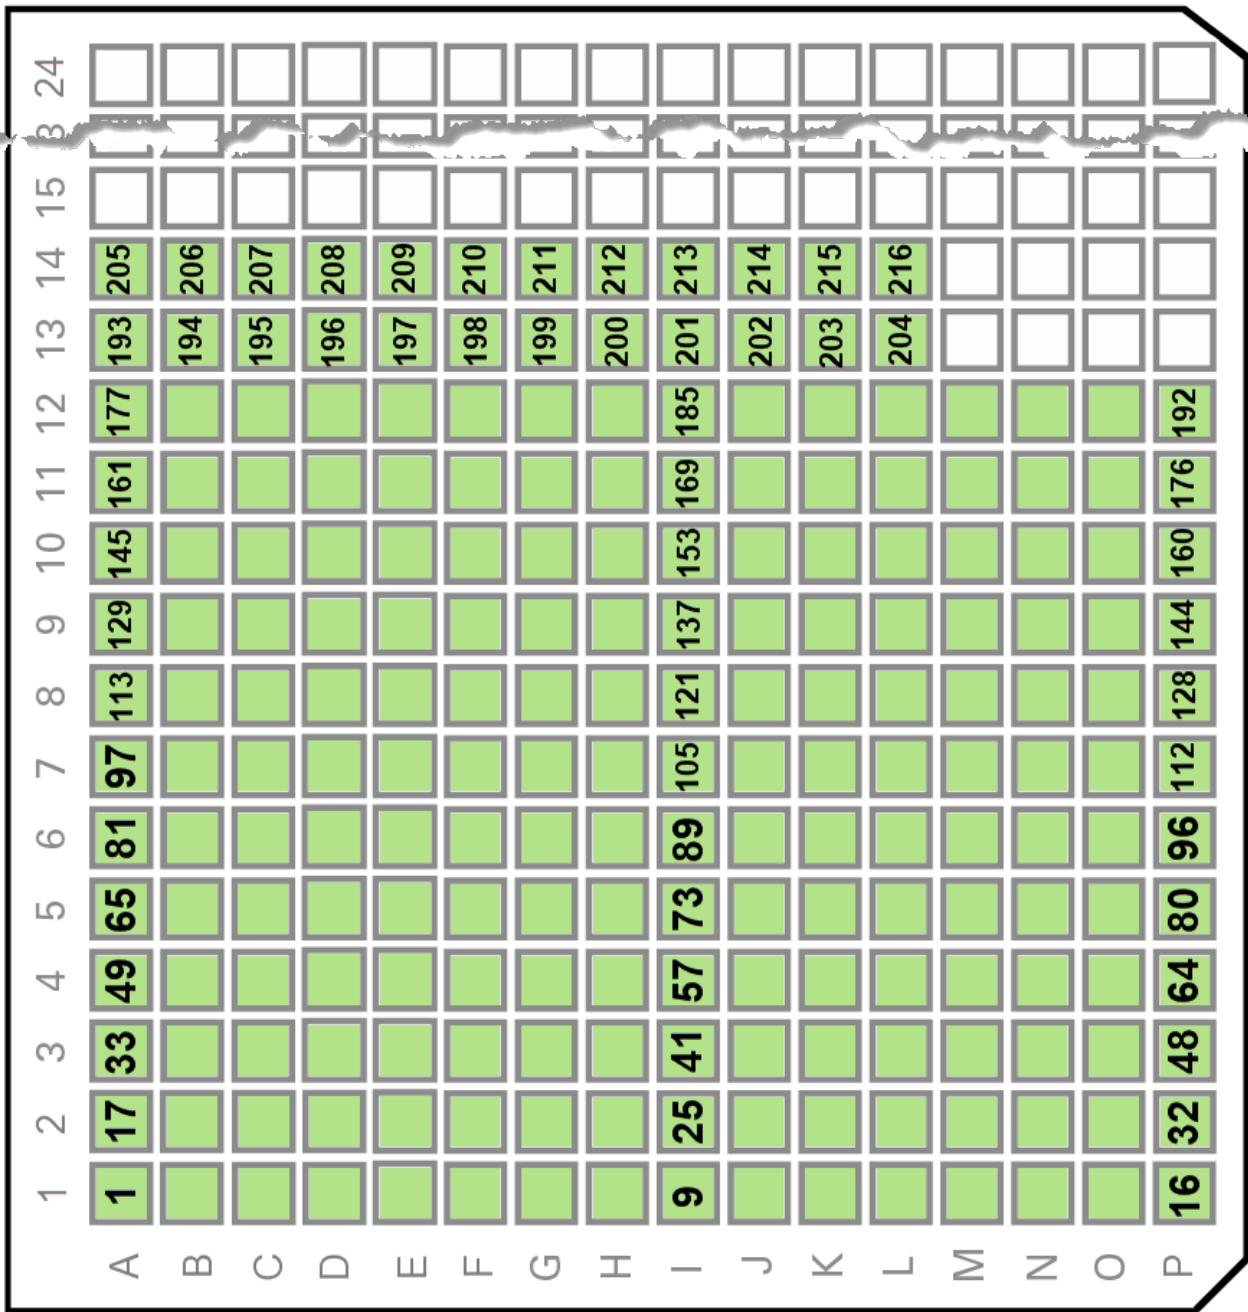


Figure 79. Printable 384-well plate map for dispense of 216 samples or assays.

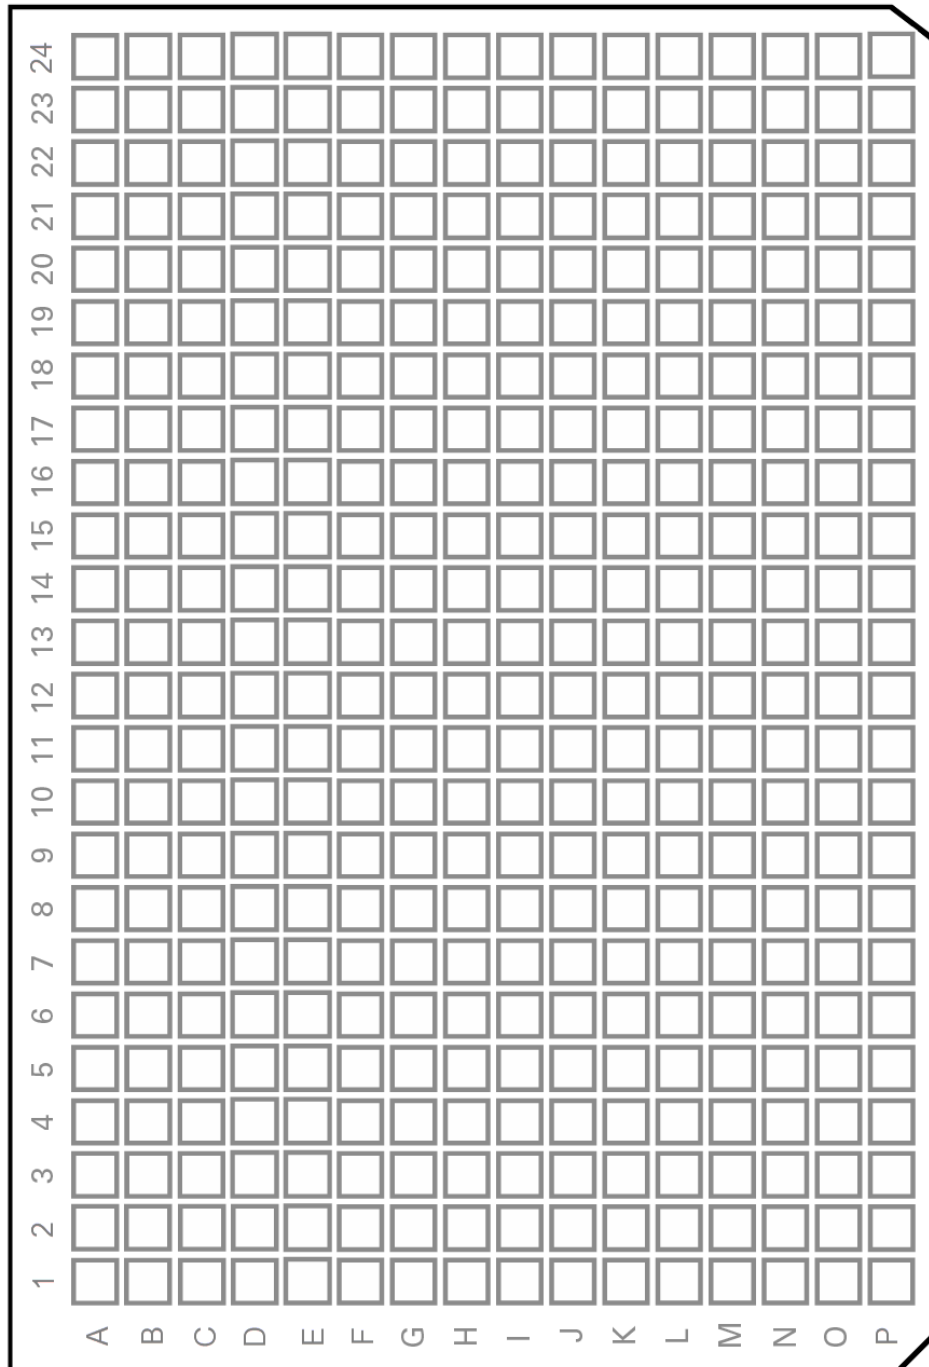


Figure 82. Printable 384-well plate map (blank).

Contact Us	
Customer Service/Ordering	Technical Support
tel: 800.662.2566 (toll-free)	tel: 800.662.2566 (toll-free)
fax: 800.424.1350 (toll-free)	fax: 800.424.1350 (toll-free)
web: takarabio.com/service	web: takarabio.com/support
e-mail: ordersUS@takarabio.com	e-mail: technical_support@takarabio.com

Notice to Purchaser

Our products are to be used for **Research Use Only**. They may not be used for any other purpose, including, but not limited to, use in humans, therapeutic or diagnostic use, or commercial use of any kind. Our products may not be transferred to third parties, resold, modified for resale, or used to manufacture commercial products or to provide a service to third parties without our prior written approval.

Your use of this product is also subject to compliance with any applicable licensing requirements described on the product's web page at takarabio.com. It is your responsibility to review, understand and adhere to any restrictions imposed by such statements

© 2023 Takara Bio Inc. All Rights Reserved.

All trademarks are the property of Takara Bio Inc. or its affiliate(s) in the U.S. and/or other countries or their respective owners. Certain trademarks may not be registered in all jurisdictions. Additional product, intellectual property, and restricted use information is available at takarabio.com.

This document has been reviewed and approved by the Quality Department.